

# Tollaust Pty Ltd - Lane Cove Tunnel

Marden St and Sirius Rd Stack Air Quality  
Monitoring Validated Data Report

1 January 2022 to 31 January 2022

Ref: DR.202201.LCT

Issue Date: 8 February 2022

Report prepared by: Tim Allfrey

NATA Accredited Laboratory Number  
19660

Accredited for compliance with  
ISO/IEC 17025 – Testing

The results of the tests, calibrations  
and/or measurements included in  
this document are traceable to



**Norditech Pty Ltd**  
Unit 2/87 Station Road  
Seven Hills NSW 2147

1300 572 822

[info@norditech.com.au](mailto:info@norditech.com.au)

[www.norditech.com.au](http://www.norditech.com.au)

## Document Control

Revision	Date	Details	Prepared By	Approved By
0	8/02/2022	Final	TA	BN

Prepared by



Tim Allfrey  
 8 February 2022

Approved by



Bruno Nourdine  
 8 February 2022

## Distribution

Format	Recipient	Details
PDF	Liam O'Grady	logrady@transurban.com
PDF	Colin Rymer	CRymer@transurban.com
PDF	Scott Tinsley	STinsley@transurban.com
PDF	Josh Gorham	JGorham@transurban.com

# Table of Contents

1	Executive Summary.....	5
1.1	Compliance to limits .....	5
2	Compliance Limits .....	6
2.1	Standards Compliance .....	6
3	Introduction.....	7
4	Explanation of Monitoring .....	8
4.1	Methodology.....	8
4.2	Ventilation Stacks.....	9
4.3	Data Collection .....	10
4.4	Data Validation .....	10
4.5	Reporting and Calculations.....	11
4.5.1	Data Availability .....	11
4.5.2	Unit Conversions .....	11
4.5.3	Combined Sirius Road South and Sirius Road North results .....	12
4.5.4	Accumulative Load .....	12
5	Calibrations and Maintenance .....	13
5.1	Units and Uncertainties .....	13
5.2	Last Calibrations and Maintenance performed.....	14
5.3	Maintenance Notes .....	15
5.3.1	Marden St.....	15
5.3.2	Sirius Rd South .....	15
5.3.3	Sirius Rd North .....	15
5.4	Automatic Instrument Calibration Checks .....	16
6	Results .....	17
6.1	Data Availability.....	17
6.2	Exceedances.....	18
6.3	Tabulated Results .....	19
6.3.1	Summary of 30 minute Average Data Marden St and Sirius Rd Combined .....	19
6.3.2	Summary of 30 minute Average Flow, Relative Humidity and Temperature. ....	20
6.3.3	Accumulative Load (Combined Stacks) .....	21
6.4	Graphical Representations .....	22
6.4.1	Monthly Summaries.....	22
6.4.1.1	Marden St Stack - Monthly CO .....	22
6.4.1.2	Marden St Stack - Monthly NO <sub>x</sub> .....	23
6.4.1.3	Marden St Stack – Monthly PM <sub>10</sub> .....	24
6.4.1.4	Marden St Stack – Monthly VOC .....	25
6.4.1.5	Sirius Rd Stack - Monthly CO .....	26
6.4.1.6	Sirius Rd Stack - Monthly NO <sub>x</sub> .....	27
6.4.1.7	Sirius Rd Stack – Monthly PM <sub>10</sub> .....	28
6.4.1.8	Sirius Rd Stack – Monthly VOC .....	29
6.4.2	Accumulative Loads .....	30
6.4.2.1	Combined Stacks CO Accumulative Load .....	30
6.4.2.2	Combined Stacks NO <sub>x</sub> Accumulative Load.....	31
6.4.2.3	Combined Stacks PM <sub>10</sub> Accumulative Load .....	32
6.4.2.4	Combined Stacks VOC Accumulative Load.....	33
6.4.3	Three Monthly Trends .....	34
6.4.3.1	Marden St Stack – Three Monthly CO .....	34
6.4.3.2	Marden St Stack – Three Monthly NO <sub>2</sub> , NO <sub>x</sub> .....	35
6.4.3.3	Marden St Stack – Three Monthly PM <sub>10</sub> .....	36
6.4.3.4	Marden St Stack – Three Monthly VOC.....	37
6.4.3.5	Sirius Rd Stack – Three Monthly CO .....	38
6.4.3.6	Sirius Rd Stack – Three Monthly NO <sub>2</sub> , NO <sub>x</sub> .....	39

6.4.3.7	Sirius Rd Stack – Three Monthly PM <sub>10</sub> .....	40
6.4.3.8	Sirius Rd Stack – Three Monthly VOC.....	41
7	Report Summary .....	42
	Appendix 1 .....	43
	Glossary.....	43
	Data Validation Explanations .....	43

## Figures

Figure 1:	Lane Cove Tunnel ventilation stack locations .....	9
Figure 2:	Marden St Stack – Monthly CO .....	22
Figure 3:	Marden St Stack – Monthly NO <sub>x</sub> .....	23
Figure 4:	Marden St Stack – Monthly PM <sub>10</sub> .....	24
Figure 5:	Marden St Stack – Monthly VOC .....	25
Figure 6:	Sirius Rd Stack – Monthly CO .....	26
Figure 7:	Sirius Rd Stack – Monthly NO <sub>x</sub> .....	27
Figure 8:	Sirius Rd Stack – Monthly PM <sub>10</sub> .....	28
Figure 9:	Sirius Rd Stack – Monthly VOC .....	29
Figure 10:	Combined Stacks CO Accumulative Load .....	30
Figure 11:	Combined Stacks NO <sub>x</sub> Accumulative Load .....	31
Figure 12:	Combined Stacks PM <sub>10</sub> Accumulative Load.....	32
Figure 13:	Combined Stacks VOC Accumulative Load .....	33
Figure 14:	Marden St Stack – Three Monthly CO .....	34
Figure 15:	Marden St Stack – Three Monthly NO <sub>x</sub> .....	35
Figure 16:	Marden St Stack – Three Monthly PM <sub>10</sub> .....	36
Figure 17:	Marden St Stack – Three Monthly VOC .....	37
Figure 18:	Sirius Rd Stack – Three Monthly CO .....	38
Figure 19:	Sirius Rd Stack – Three Monthly NO <sub>x</sub> .....	39
Figure 20:	Sirius Rd Stack – Three Monthly PM <sub>10</sub> .....	40
Figure 21:	Sirius Rd Stack – Three Monthly VOC.....	41

## Tables

Table 1: Exceedances of MCoA Goals .....	5
Table 2: MCoA Compliance Goals.....	6
Table 3: Measurement methods and instrumentation .....	8
Table 4: Lane Cove Tunnel ventilation stack GPS Coordinates .....	9
Table 5: Sirius Rd Reporting Condition criteria .....	12
Table 6: Measurement units and uncertainties .....	13
Table 7: Instrument details and calibration dates.....	14
Table 8: Nightly span, zero and CO reference times.....	16
Table 9: LCT ventilation stack data availability .....	17
Table 10: Exceedances of MCoA Goals .....	18
Table 11: Summary of 30 minute average data Marden St and Sirius Rd combined.....	19
Table 12: Summary of 30 minute average flow, RH and temperature .....	20
Table 13: Total Accumulative Load (Combined Stacks).....	21

# 1 Executive Summary

The Lane Cove Tunnel runs for 3.6km between North Ryde and Artarmon, linking the M2 Motorway and the Gore Hill Freeway and forms part of Sydney’s motorway network. The tunnel commenced operation in March 2007.

Two stacks provide ventilation for the tunnel, one at the western end of the tunnel (Sirius Road, Lane Cove West), and one at the eastern end of the tunnel (Marden St, Artarmon). The Sirius Road stack comprises two partitions, north and south. Sirius Road results are a combined weighted average to the two partitions.

This report presents the monthly validated stack data for January 2022 to Tollaust Pty Ltd for the Lane Cove Tunnel.

## 1.1 Compliance to limits

The Minister’s Conditions of Approval (MCoA) designates limits to which pollutants being discharged from the ventilation stacks must meet. (MCoA 173).

There were nil exceedances of the prescribed limits during the reporting period.

Lane Cove Tunnel Ventilation Stack Air Quality Limit Exceedances January 2022							
Location	Parameter	Time Period	Concentration Limit	Units	Number of exceedances	Value of exceedance	Date and Time of exceedance
Marden St (Eastern Stack)	CO	30 minutes	62.5	mg/m <sup>3</sup>	0	-	-
	NO <sub>x</sub>	30 minutes	25.7	mg/m <sup>3</sup>	0	-	-
	PM <sub>10</sub>	30 minutes	1200	µg/m <sup>3</sup>	0	-	-
	VOC	30 minutes	6.3	mg/m <sup>3</sup>	0	-	-
Sirius Rd (Western Stack)	CO	30 minutes	62.5	mg/m <sup>3</sup>	0	-	-
	NO <sub>x</sub>	30 minutes	32.8	mg/m <sup>3</sup>	0	-	-
	PM <sub>10</sub>	30 minutes	1600	µg/m <sup>3</sup>	0	-	-
	VOC	30 minutes	6.3	mg/m <sup>3</sup>	0	-	-
Combined Stacks	CO	Annual	1530	t/annum	0	-	-
	NO <sub>x</sub>	Annual	229	t/annum	0	-	-
	PM <sub>10</sub>	Annual	14	t/annum	0	-	-
	VOC	Annual	153	t/annum	0	-	-

Table 1: Exceedances of MCoA Goals

For further information relating to exceedance reporting please refer to sections Compliance Limits, and Exceedances.

## 2 Compliance Limits

Air quality goals provided are provided in Condition 173 of the Minister's Conditions of Approval issued by the Director-General for the Lane Cove Tunnel project. The air quality goals are shown in the table below.

Lane Cove Tunnel Ventilation Stack Air Quality Limits					
Location	Parameter	Time Period	Concentration Limit	Units	Applicable MCoA
Marden St (Eastern Stack)	CO	30 minutes	62.5	mg/m <sup>3</sup>	MCoA 173
	NO <sub>x</sub>	30 minutes	25.7	mg/m <sup>3</sup>	MCoA 173
	PM <sub>10</sub>	30 minutes	1200	µg/m <sup>3</sup>	MCoA 173
	VOC	30 minutes	6.3	mg/m <sup>3</sup>	MCoA 173
Sirius Rd (Western Stack)	CO	30 minutes	62.5	mg/m <sup>3</sup>	MCoA 173
	NO <sub>x</sub>	30 minutes	32.8	mg/m <sup>3</sup>	MCoA 173
	PM <sub>10</sub>	30 minutes	1600	µg/m <sup>3</sup>	MCoA 173
	VOC	30 minutes	6.3	mg/m <sup>3</sup>	MCoA 173
Combined Stacks	CO	Annual	1530	t/annum	MCoA 173
	NO <sub>x</sub>	Annual	229	t/annum	MCoA 173
	PM <sub>10</sub>	Annual	14	t/annum	MCoA 173
	VOC	Annual	153	t/annum	MCoA 173

Table 2: MCoA Compliance Goals

### 2.1 Standards Compliance

Norditech's NATA Accreditation does not cover the following parameters monitored at the Lane Cove Tunnel stack air quality monitoring stations

- Measurement of Stack Flow.
- Particulate matter PM<sub>10</sub> and PM<sub>2.5</sub> sampled by means of an isokinetic sampling system
- AS/NZS 3580.9.8 refers specifically to the monitoring of PM<sub>10</sub>.

### 3 Introduction

Norditech were contracted by Tollaust Pty Ltd in December 2018 to provide continuous stack air quality monitoring and reporting services for Lane Cove Tunnel.

Norditech is a NATA accredited organisation (Accreditation Number 19660)

Addresses of relevant parties:

**Norditech Pty Ltd**  
2/87 Station Rd  
Seven Hills NSW 2147

**Tollaust Pty Ltd**  
5 Sirius Rd  
Lane Cove West NSW 2066

This report presents the validated Marden St and Sirius Rd ventilation stack data for January 2022.

- Describes air quality measurements.
- Reports any readings above the LCT Limits.
- Compares monitoring results.
- Has been quality assured.



## 4 Explanation of Monitoring

### 4.1 Methodology

In tunnel air is discharged via two ventilation stacks – one located at Marden St, Artarmon, and one located at Sirius Rd, Lane Cove West. The Sirius Rd stack comprises of two separate partitions (North and South). For each stack, monitoring as per the requirements of MCoA 172 is undertaken. Each partition of the Sirius Rd stack is monitored by separate air quality monitoring stations.

Gaseous parameters are sampled by an extractive sampling system with automatic purging. Volatile organic compounds are measured using the flame ionization detection principle. Oxides of nitrogen are measured using chemiluminescence. Carbon monoxide is measured using non-dispersive infra-red absorption.

Particulates PM<sub>10</sub> and PM<sub>2.5</sub> are measured using tapered element oscillating microbalances, via an isokinetic sampling system.

Monthly routine maintenance is undertaken by Norditech. Maintenance is performed as per the relevant Australian Standard or in house method. Maintenance cycles generally involve 1, 3, 6 and 12 monthly scheduled items.

The following instrumentation and methods are used data collection:

LCT Ventilation Stack Measurement Methods		
Parameter	Method	Instrument
CO	In house method TP.003	Ecotech Serinus S30
NO, NO <sub>2</sub> , NO <sub>x</sub>	In house method TP.001	Ecotech Serinus S40
CH <sub>4</sub> , NMHC, VOC	In house method TP.006	Baseline 9000, ENVEA HC51M
PM <sub>10</sub>	AS/NZS 3580.9.8	Rupprecht & Patashnick TEOM with Ecotech and Norditech ISS isokinetic sampling system
	In house method TP.005	
	AS 4323.1	
PM <sub>2.5</sub>	In house method TP.026	Rupprecht & Patashnick TEOM with Ecotech and Norditech ISS isokinetic sampling system
	AS 4323.1	
Temperature	In house method TP.012	Vaisala HMT330
Relative Humidity	In house method TP.014	Vaisala HMT330
Flow Rate	TBA	Flowsic 100 USD 55SSTI Ultrasonic flow sensor

Table 3: Measurement methods and instrumentation

## 4.2 Ventilation Stacks

The locations of the Marden St and Sirius Rd ventilation stacks are detailed in the table and figure below.

LCT Tunnel Ventilation Stack Locations	
Parameter	GPS Coordinates
Marden St (Eastern Stack)	-33.815025°, 151.179246°
Sirius Rd (Western Stack)	-33.807887°, 151.146074°

Table 4: Lane Cove Tunnel ventilation stack GPS Coordinates

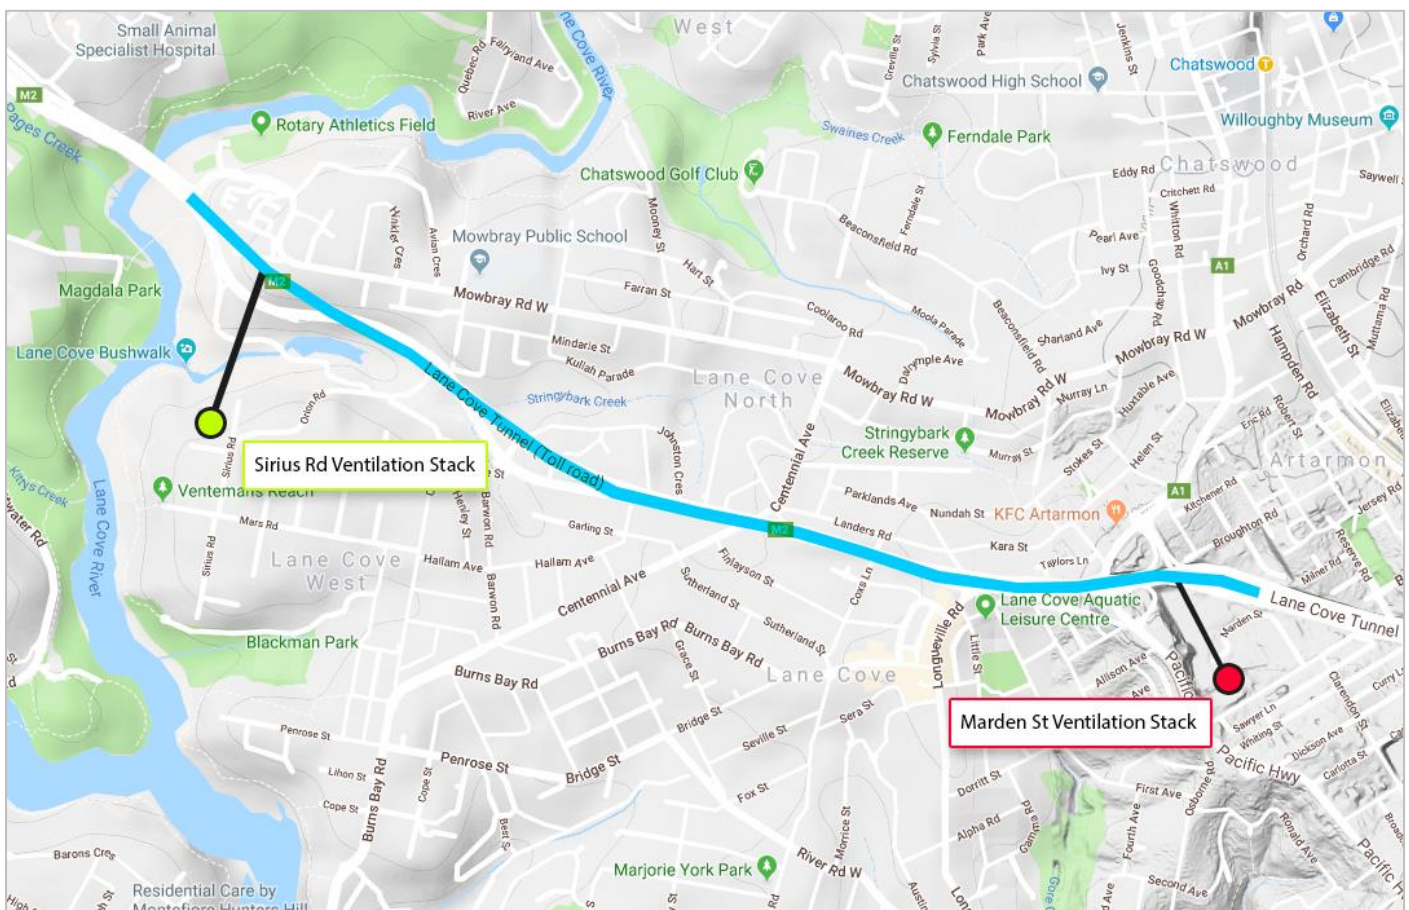


Figure 1: Lane Cove Tunnel ventilation stack locations

## 4.3 Data Collection

At each Air Quality Monitoring Station, data is logged to a WinAQMS data logger at 5 minute average intervals. Each 5 minute average is calculated from data sampled at 10 second intervals.

Data is transferred automatically to Norditech's data collection software via a TCP/IP link over ADSL, at a frequency of not less than 1 hour. Two datasets are maintained by Norditech, one for data validation and reporting purposes, and a non-validated data set for reference purposes.

Transurban also keeps a non-validated data set on the Airodis data collection PC located at the Lane Cove Tunnel Control Room. This PC is maintained by Norditech.

## 4.4 Data Validation

Data validation is performed as per Norditech's data validation procedure TP.022. The data validation process identifies any data that is deemed not to be valid. This data is flagged as invalid in the database and is removed from the reported data.

Data may be deemed invalid for several reasons, including but not limited to:

- Instrument fault
- Instrument calibration out of tolerance
- Maintenance activities

For further details and explanations of reasons for invalidating data, please refer to Appendix 1 – Data Validation Explanations.

Initial visual inspection of data is performed by inspection of graphs to identify any anomalies in the data set.

Site visit logs and maintenance and calibration certificates are cross referenced to the data set and any data affected by maintenance activities are flagged.

Instrument drift and calibration tolerances are checked and data flagged in the database as necessary as per NATA compliance requirements.

## 4.5 Reporting and Calculations

All calculations and averages are calculated from 5 minute average base data and are reported as 'end time'. IE the average data for 01:05 is the data from 01:00 through to 01:05.

Validated data for Marden St Stack is presented in the Excel workbook named "202201 LCT Marden St Stack Validated data.xlsx". The workbook consists of the following sheets:

1. Cover
2. Marden St 5m Avg
3. Marden St Span Zero Data
4. Marden St Data Validation

Validated data for Sirius Rd Stack is presented in the Excel workbook named "202201 LCT Sirius Rd Stack Validated data.xlsx". The workbook consists of the following sheets:

1. Cover
2. Sirius Rd Combined 5m Avg
3. Flow Temp RH Individual 5m Avg
4. Sirius Rd South Span Zero Data
5. Sirius Rd North Span Zero Data
6. Sirius Rd South Data Validation
7. Sirius Rd North Data Validation

### 4.5.1 Data Availability

Data availability refers to the amount of available data for the reporting period. Data availability is calculated using the following formula:

$$\text{Data availability \%} = \frac{\text{sum of available data points}}{\text{sum of possible data points}} * 100$$

Where:

- Sum of available data points is the number of validated 5 minute average data points for the reporting period
- Sum of possible data points is the number of theoretically available data points for the reporting period

### 4.5.2 Unit Conversions

Total oxides of nitrogen (NO<sub>x</sub>) results are expressed as NO<sub>2</sub> equivalents in mg/m<sup>3</sup>. As of 1/03/2021, VOC results are expressed as non-methane hydrocarbons as propane equivalents in mg/m<sup>3</sup>. Prior to this date VOC results were expressed as total VOCs as methane equivalent.

Stack velocity readings are converted to flow rate using the following stack areas:

- Marden Street Stack area 59.8919 m<sup>2</sup>
- Sirius Road Stack – North Partition area 35.95 m<sup>2</sup>
- Sirius Road Stack – South Partition area 36.19 m<sup>2</sup>

Pollutant and flow data are reported at reference conditions: 0°C, 101.325 kPa, dry.

### 4.5.3 Combined Sirius Road South and Sirius Road North results

Data from the Sirius Road stack are combined results of the north and south partitions. Stack velocity is used to determine whether a partition is active or inactive, and this determines the calculation for the total Sirius Road ventilation stack results.

The table below shows the criteria used to determine how the total Sirius Road ventilation stack data is calculated.

LCT Tunnel Sirius Rd Ventilation Stack Reporting Conditions	
Partitions Active	Calculation
None	Combined result is based on weighted total from both partitions. Weighting is calculated as a function of the ratio of partition flows to total flow
One	Active partition is reported
Both	Combined result is based on weighted total from both partitions. Weighting is calculated as a function of the ratio of partition flows to total flow
Unknown in either partition	No result provided as it can not be determined whether each partition is active or not.

Table 5: Sirius Rd Reporting Condition criteria

### 4.5.4 Accumulative Load

Accumulative loads are calculated from the monthly measured emission in tonnes for each stack for CO, NO<sub>x</sub>, PM<sub>10</sub> and VOC. The measured emissions are converted to an estimated monthly total emission by taking into account the data capture of each parameter, using the following formula:

$$estimated\ monthly\ total\ emission = \frac{measured\ monthly\ emission}{available\ data\ \%} * 100$$

The estimated monthly total emissions for each parameter for each stack are then added together to give the total emission per parameter per month.

The accumulative load is then calculated as the sum of the previous 12 months estimated total emission for each parameter.

If there is less than 50% data availability for any parameter, then data for the last valid previous month (i.e. above 50% data availability) is substituted.

## 5 Calibrations and Maintenance

### 5.1 Units and Uncertainties

LCT Ventilation Stack Instrument Units and Uncertainties				
Parameter	Units	Resolution	Uncertainty	Measurement Range
CO	mg/m <sup>3</sup>	0.01	± 8.2% of reading at 62.5mg/m <sup>3</sup> (k=1.96)	0 to 123
NO	mg/m <sup>3</sup>	0.01	± 8.1% of reading for range 25.7 – 32.8mg/m <sup>3</sup> (k=1.96)	0 to 31
NO <sub>2</sub>	mg/m <sup>3</sup>	0.01	± 8.5% of reading at 25.7mg/m <sup>3</sup> (k=1.96)	0 to 33
NO <sub>x</sub>	mg/m <sup>3</sup>	0.01	± 8.1% of reading for range 25.7 – 32.8mg/m <sup>3</sup> (k=1.96)	0 to 33
CH <sub>4</sub>	mg/m <sup>3</sup>	0.01	±12% of reading + 0.3mg/m <sup>3</sup> for range 3.5 – 17mg/m <sup>3</sup> (k=2.0)	0 to 17
NMHC (as propane)	mg/m <sup>3</sup>	0.01	±13% of reading + 0.56mg/m <sup>3</sup> for range 3.5 – 20mg/m <sup>3</sup> (k=2.0)	0 to 20
PM <sub>10</sub>	µg/m <sup>3</sup>	0.1	±5.0 µg/m <sup>3</sup> or 3.6% of reading, whichever is the greater. K factor of 1.96	0 to 5000
PM <sub>2.5</sub>	µg/m <sup>3</sup>	0.1	±5.0 µg/m <sup>3</sup> or 3.6% of reading, whichever is the greater. K factor of 1.96	0 to 5000
Temperature	°C	0.1	± 0.6°C, K factor of 2.0	0 to 50
Relative Humidity	%	1	± 6%, K factor of 2.0	1 to 100
Flow Rate	m <sup>3</sup> /s	1	±0.1 for velocity measurement <sup>1</sup>	-40 to +40

<sup>1</sup> Manufacturer's stated accuracy

Table 6: Measurement units and uncertainties

## 5.2 Last Calibrations and Maintenance performed

Instrumentation maintenance and last calibration dates are provided in the table below

LCT Stack Maintenance and Calibrations January 2022				
Location	Parameter	Date of last maintenance	Maintenance type	Date of last calibration
Marden St	CO	10/01/2022	1 Monthly	10/01/2022
	NO, NO2, NOx	10/01/2022	1 Monthly	10/01/2022
	VOC	10/01/2022	1 Monthly	10/01/2022
	PM10	10/01/2022	1 Monthly	17/11/2021
	PM2.5	10/01/2022	1 Monthly	17/11/2021
	Temperature	31/08/2021	12 Monthly	31/08/2021
	Relative Humidity	31/08/2021	12 Monthly	31/08/2021
	Flow Rate	N/A	N/A	15/07/2020
Sirius Rd South	CO	27/01/2022	12 Monthly	27/01/2022
	NO, NO2, NOx	27/01/2022	12 Monthly	27/01/2022
	VOC	27/01/2022	12 Monthly	27/01/2022
	PM10	28/01/2022	12 Monthly	28/01/2022
	PM2.5	28/01/2022	12 Monthly	28/01/2022
	Temperature	28/01/2022	12 Monthly	28/01/2022
	Relative Humidity	28/01/2022	12 Monthly	28/01/2022
	Flow Rate	N/A	N/A	15/07/2020
Sirius Rd North	CO	12/01/2022	1 Monthly	12/01/2022
	NO, NO2, NOx	12/01/2022	1 Monthly	12/01/2022
	VOC	12/01/2022	1 Monthly	12/01/2022
	PM10	12/01/2022	1 Monthly	4/11/2021
	PM2.5	12/01/2022	1 Monthly	4/11/2021
	Temperature	19/08/2021	6 Monthly	19/08/2021
	Relative Humidity	19/08/2021	6 Monthly	19/08/2021
	Flow Rate	N/A	N/A	15/07/2020

Table 7: Instrument details and calibration dates

## 5.3 Maintenance Notes

The sections below describe the major maintenance undertaken at each of the three monitoring stations during the reporting period. For further details please refer to the corresponding data validation table contained within the relevant accompanying data report file.

### 5.3.1 Marden St

- Scheduled maintenance was undertaken on 10/01/2022

### 5.3.2 Sirius Rd South

- Scheduled maintenance was undertaken on 27/01/2022 and 28/01/2022

### 5.3.3 Sirius Rd North

- Scheduled maintenance was undertaken on 12/01/2022



## 5.4 Automatic Instrument Calibration Checks

The table below identifies the times at which the daily gaseous parameter automatic span and zero checks are performed.

Further to the span and zero checks, the CO analysers perform nightly background reference cycles.

This data is removed from the dataset, however are not included in the data validation tables.

Nightly span and zero times for NO, NO <sub>2</sub> , NO <sub>x</sub> , CO, CH <sub>4</sub> and NMHC			
Location	Parameter	Span / Zero cycle time	Background cycle time
Marden St	CO	1:00 - 2:00	23:45 - 23:50
	NO, NO <sub>2</sub> , NO <sub>x</sub>	1:00 - 2:00	-
	VOC	1:00 - 2:00	-
Sirius Rd South	CO	1:00 - 2:00	23:45 - 23:50
	NO, NO <sub>2</sub> , NO <sub>x</sub>	1:00 - 2:00	-
	VOC	1:00 - 2:00	-
Sirius Rd North	CO	1:00 - 2:00	23:45 - 23:50
	NO, NO <sub>2</sub> , NO <sub>x</sub>	1:00 - 2:00	-
	VOC	1:00 - 2:00	-

Table 8: Nightly span, zero and CO reference times.

## 6 Results

### 6.1 Data Availability

Data availability for the ventilation stack parameters are provided in the table below. Locations with data availability less than 90% are indicated in red italics.

- Data availability for all parameters measured in the Lane Cove Tunnel Marden St stack were above 90% for the reporting period with the exception of CO and VOC.
- Data availability for all parameters measured in the Lane Cove Tunnel Sirius Rd stack were below 90% for the reporting period with the exception of PM10.

LCT Ventilation Stack Data Capture January 2022								
Station	CO (%)	NO (%)	NO <sub>2</sub> (%)	NO <sub>x</sub> (%)	PM <sub>10</sub> (%)	PM <sub>2.5</sub> (%)	VOC (%)	Flow (%)
Marden St Stack	<i>80.7</i>	93.2	93.6	93.6	96.4	95.3	<i>78.4</i>	99.7
Sirius Rd Stack	<i>86.6</i>	<i>78.3</i>	<i>78.3</i>	<i>78.3</i>	94.8	<i>85.6</i>	<i>78.3</i>	96.0

Table 9: LCT ventilation stack data availability

## 6.2 Exceedances

Instances of the ventilation stack pollutants exceeding the MCoA goals during the reporting period are presented in the table below.

There were nil exceedances of the prescribed limits during the reporting period.

Lane Cove Tunnel Ventilation Stack Air Quality Limit Exceedances January 2022							
Location	Parameter	Time Period	Concentration Limit	Units	Number of exceedances	Value of exceedance	Date and Time of exceedance
Marden St (Eastern Stack)	CO	30 minutes	62.5	mg/m <sup>3</sup>	0	-	-
	NO <sub>x</sub>	30 minutes	25.7	mg/m <sup>3</sup>	0	-	-
	PM <sub>10</sub>	30 minutes	1200	µg/m <sup>3</sup>	0	-	-
	VOC	30 minutes	6.3	mg/m <sup>3</sup>	0	-	-
Sirius Rd (Western Stack)	CO	30 minutes	62.5	mg/m <sup>3</sup>	0	-	-
	NO <sub>x</sub>	30 minutes	32.8	mg/m <sup>3</sup>	0	-	-
	PM <sub>10</sub>	30 minutes	1600	µg/m <sup>3</sup>	0	-	-
	VOC	30 minutes	6.3	mg/m <sup>3</sup>	0	-	-
Combined Stacks	CO	Annual	1530	t/annum	0	-	-
	NO <sub>x</sub>	Annual	229	t/annum	0	-	-
	PM <sub>10</sub>	Annual	14	t/annum	0	-	-
	VOC	Annual	153	t/annum	0	-	-

Table 10: Exceedances of MCoA Goals

## 6.3 Tabulated Results

### 6.3.1 Summary of 30 minute Average Data Marden St and Sirius Rd Combined

The following table presents 30 minute average minimum, maximum and daily average data for the Marden St Stack, and Sirius Rd combined stack.

30 minute averages are calculated from 5 minute average data. The daily average is calculated from 30 minute average data.

LCT Ventilation Stack Summary January 2022								
Parameter	CO (mg/m <sup>3</sup> )	NO (mg/m <sup>3</sup> )	NO <sub>2</sub> (mg/m <sup>3</sup> )	NO <sub>x</sub> (mg/m <sup>3</sup> )	PM <sub>10</sub> (µg/m <sup>3</sup> )	PM <sub>2.5</sub> (µg/m <sup>3</sup> )	VOC (mg/m <sup>3</sup> )	Flow (m <sup>3</sup> /s)
Marden St (Eastern Stack)								
Minimum 30 minute average	0.17	0.01	0.03	0.04	-7.4	-9.9	0.00	5
Maximum 30 minute average	7.85	4.27	1.04	7.32	280.8	212.8	0.81	517
Average	2.76	0.93	0.22	1.64	53.4	42.2	0.18	382
Limit	62.5			25.7	1200		6.3	
Sirius Rd (Western Stack)								
Minimum 30 minute average	-0.07	0.00	0.01	0.01	-2.9	-7.1	0.03	5
Maximum 30 minute average	9.12	3.67	0.69	6.31	148.7	101.0	1.53	370
Average	1.29	0.33	0.09	0.60	31.9	22.8	0.23	340
Limit	62.5			32.8	1600		6.3	

Table 11: Summary of 30 minute average data Marden St and Sirius Rd combined

### 6.3.2 Summary of 30 minute Average Flow, Relative Humidity and Temperature.

The following table presents 30 minute average minimum, maximum and daily average flow, relative humidity, and temperature data for the Marden St Stack, and Sirius Rd North and South partitions.

30 minute averages are calculated from 5 minute average data. The daily average is calculated from 30 minute average data.

LCT Ventilation Stack Flow, RH, Temp Summary January 2022									
Parameter	Marden St (Eastern Stack)			Sirius Rd - South Partition			Sirius Rd - North Partition		
	Flow (m <sup>3</sup> /s)	RH (%)	Temp (°C)	Flow (m <sup>3</sup> /s)	RH (%)	Temp (°C)	Flow (m <sup>3</sup> /s)	RH (%)	Temp (°C)
Minimum 30 minute average	5	36	23.2	3	25	21.2	1	44	19.2
Maximum 30 minute average	517	81	30.8	355	91	39.1	352	90	30.1
Average	382	61	27.3	288	62	26.8	51	69	24.1

Table 12: Summary of 30 minute average flow, RH and temperature

### 6.3.3 Accumulative Load (Combined Stacks)

The following table presents annual accumulative total loads for CO, NO<sub>x</sub>, PM<sub>10</sub> and VOC.

Where data availability is less than 50%, data has been substituted with data from the last valid monthly accumulated load for that parameter (i.e. the last month for which greater than 50% of data was available).

LCT Stack Accumulative Load February 2021 to January 2022				
	Carbon Monoxide	Oxides of Nitrogen	PM <sub>10</sub>	VOC
	Tonnes	Tonnes	Tonnes	Tonnes
Accumulative Load for past 12 months	52.6	37.1	1.2	8.0
Annual Limit (Tonnes)	1530	229	14	153

Table 13: Total Accumulative Load (Combined Stacks)

## 6.4 Graphical Representations

### 6.4.1 Monthly Summaries

The following charts present 30 minute average minimum, maximum and daily average data CO, NO<sub>x</sub>, PM<sub>10</sub> and VOC for the Marden St Stack, and Sirius Rd combined stack.

30 minute averages are calculated from 5 minute average data. The daily average is calculated from 30 minute average data.

#### 6.4.1.1 Marden St Stack - Monthly CO

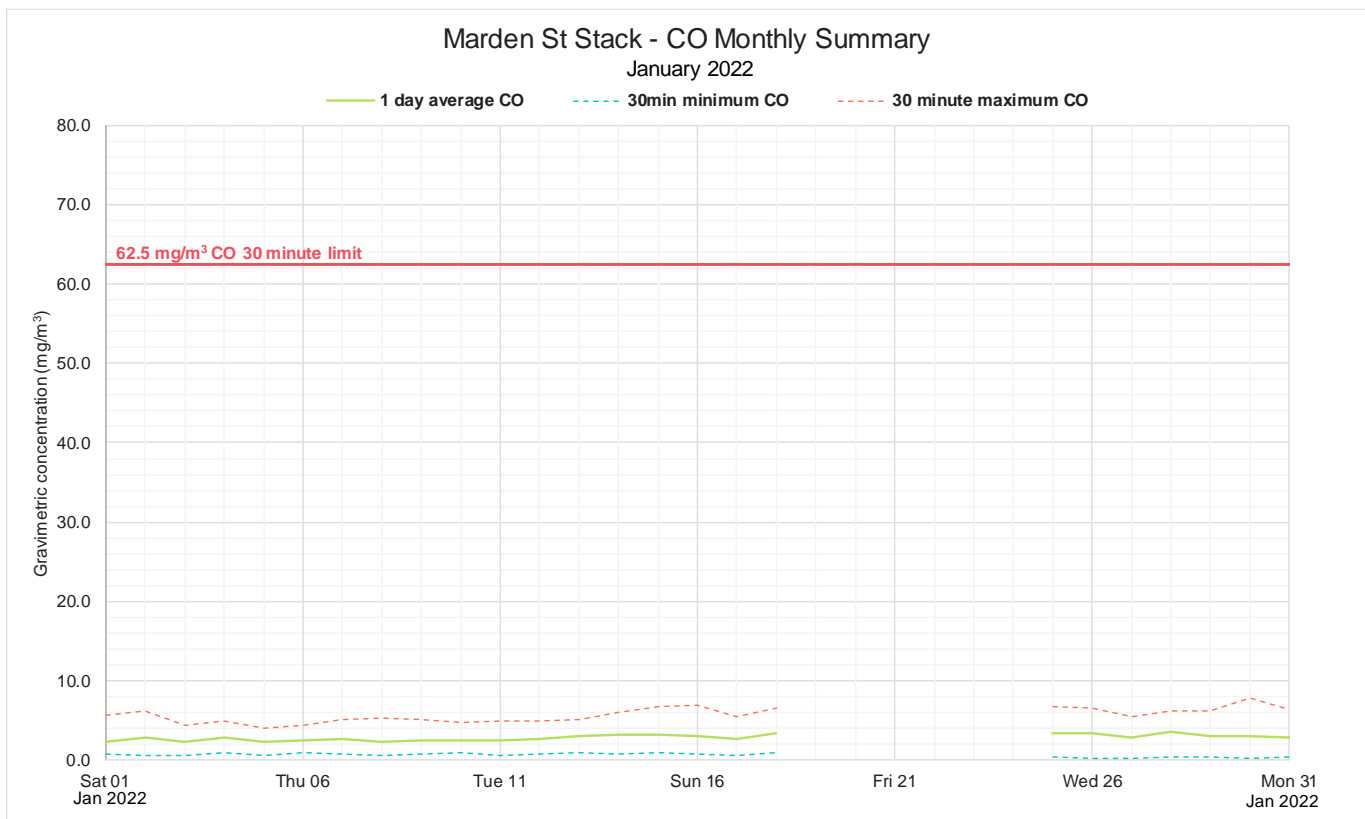


Figure 2: Marden St Stack – Monthly CO

6.4.1.2 Marden St Stack - Monthly NO<sub>x</sub>

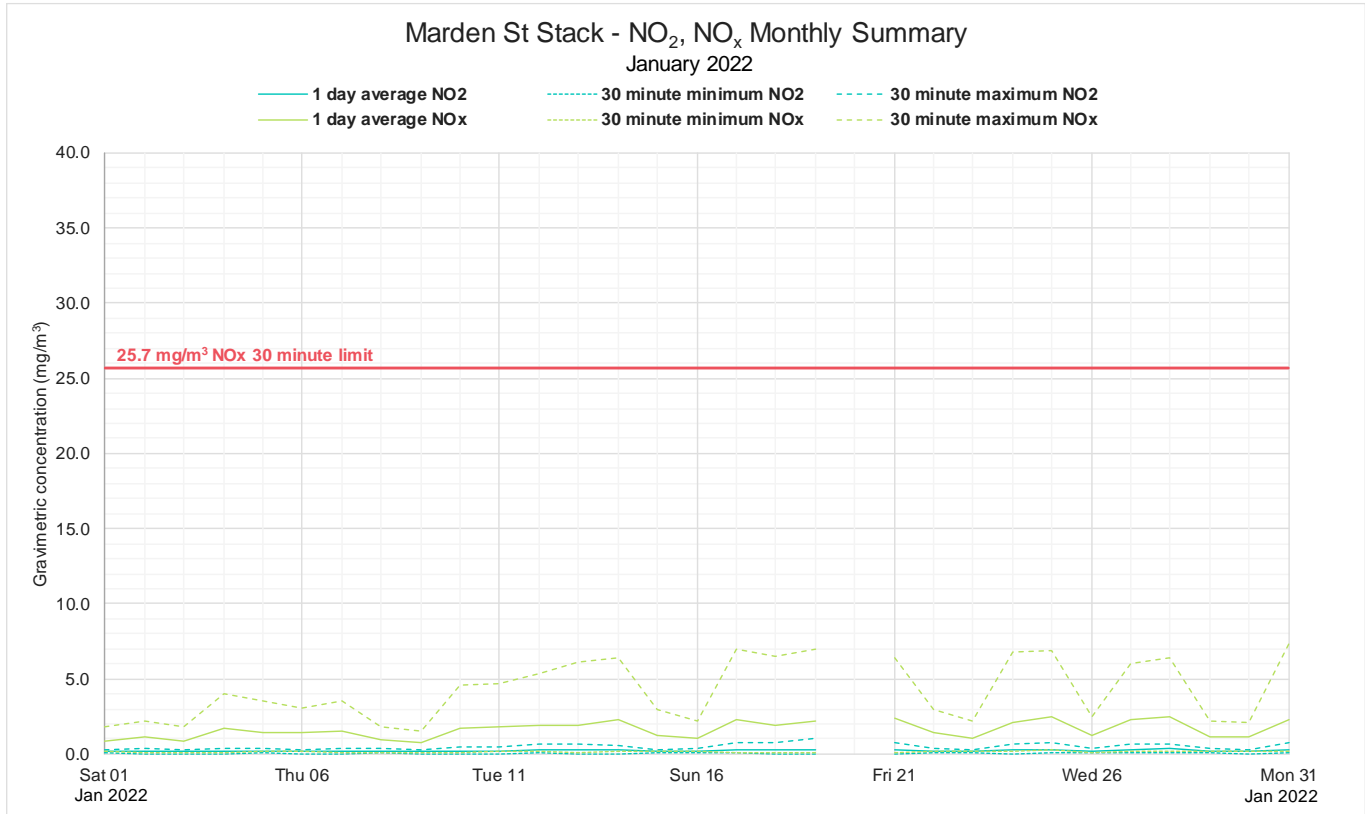


Figure 3: Marden St Stack – Monthly NO<sub>x</sub>



6.4.1.3 Marden St Stack – Monthly PM<sub>10</sub>

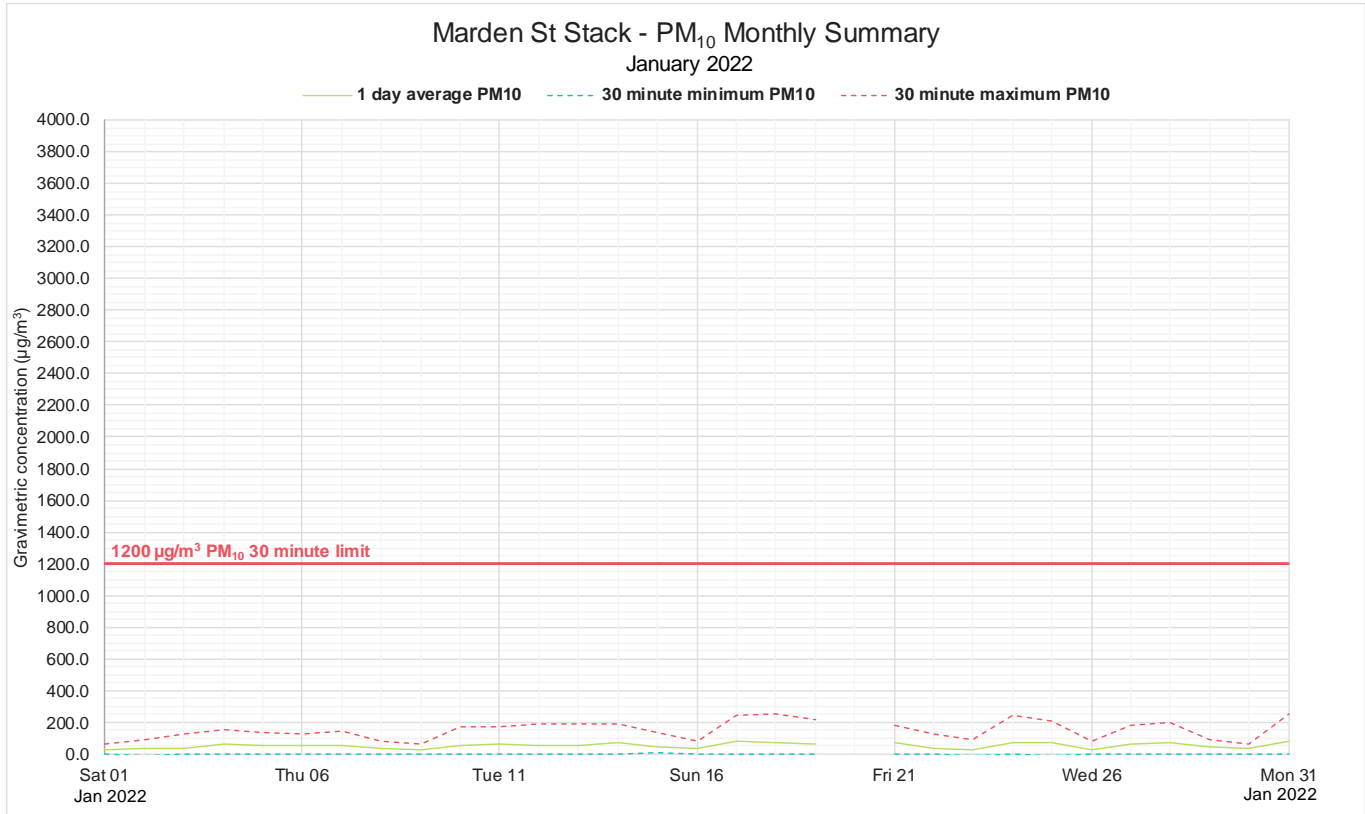


Figure 4: Marden St Stack – Monthly PM<sub>10</sub>

6.4.1.4 Marden St Stack – Monthly VOC

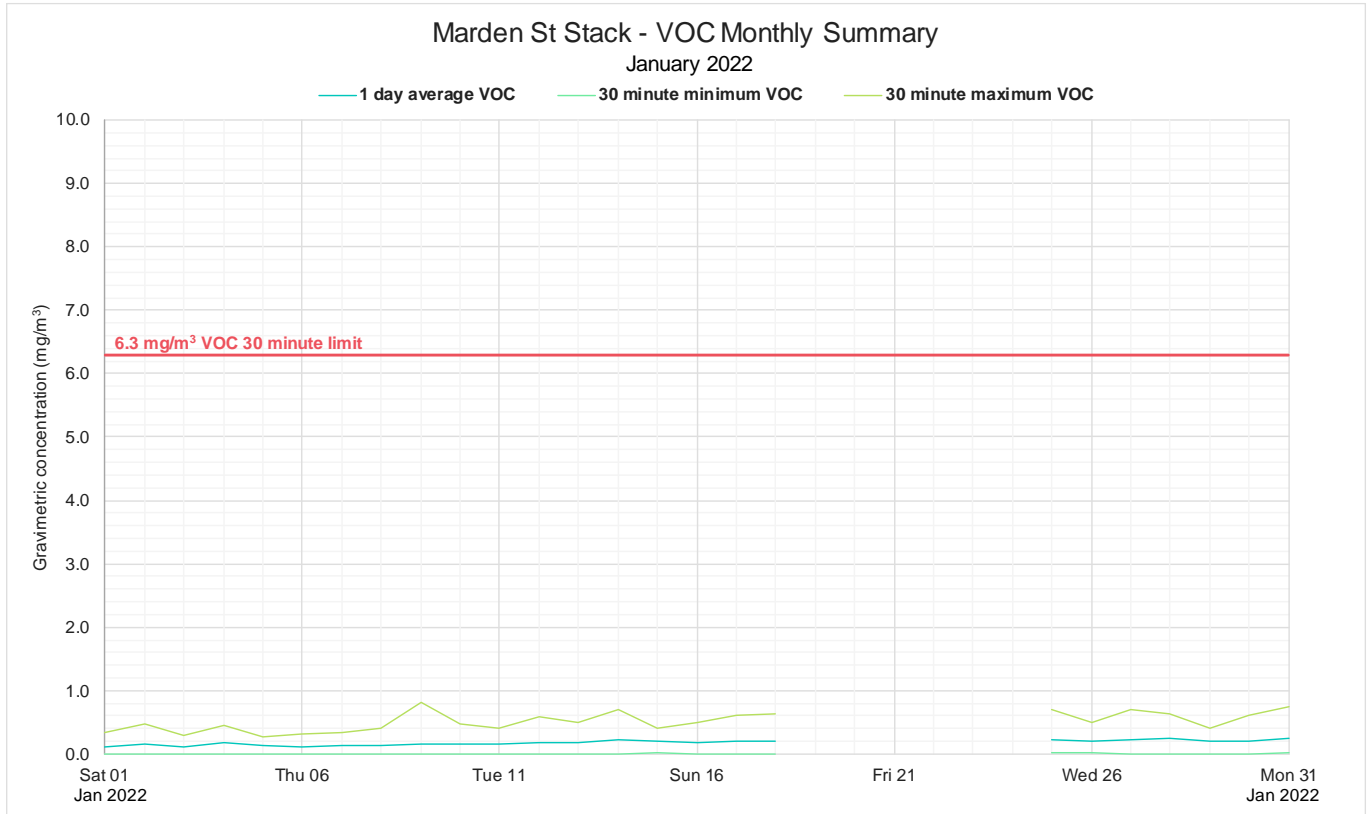


Figure 5: Marden St Stack – Monthly VOC

6.4.1.5 Sirius Rd Stack - Monthly CO

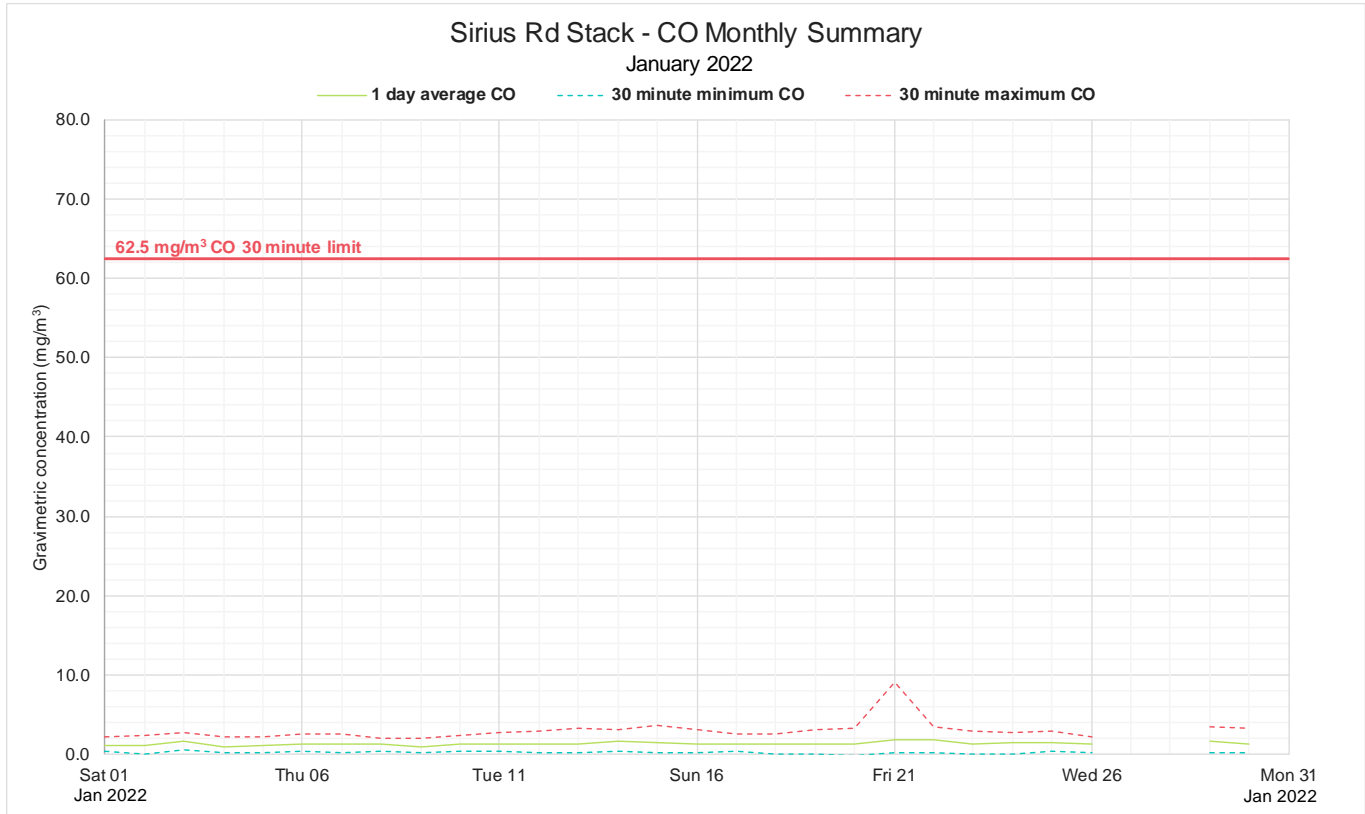


Figure 6: Sirius Rd Stack – Monthly CO

6.4.1.6 Sirius Rd Stack - Monthly NO<sub>x</sub>

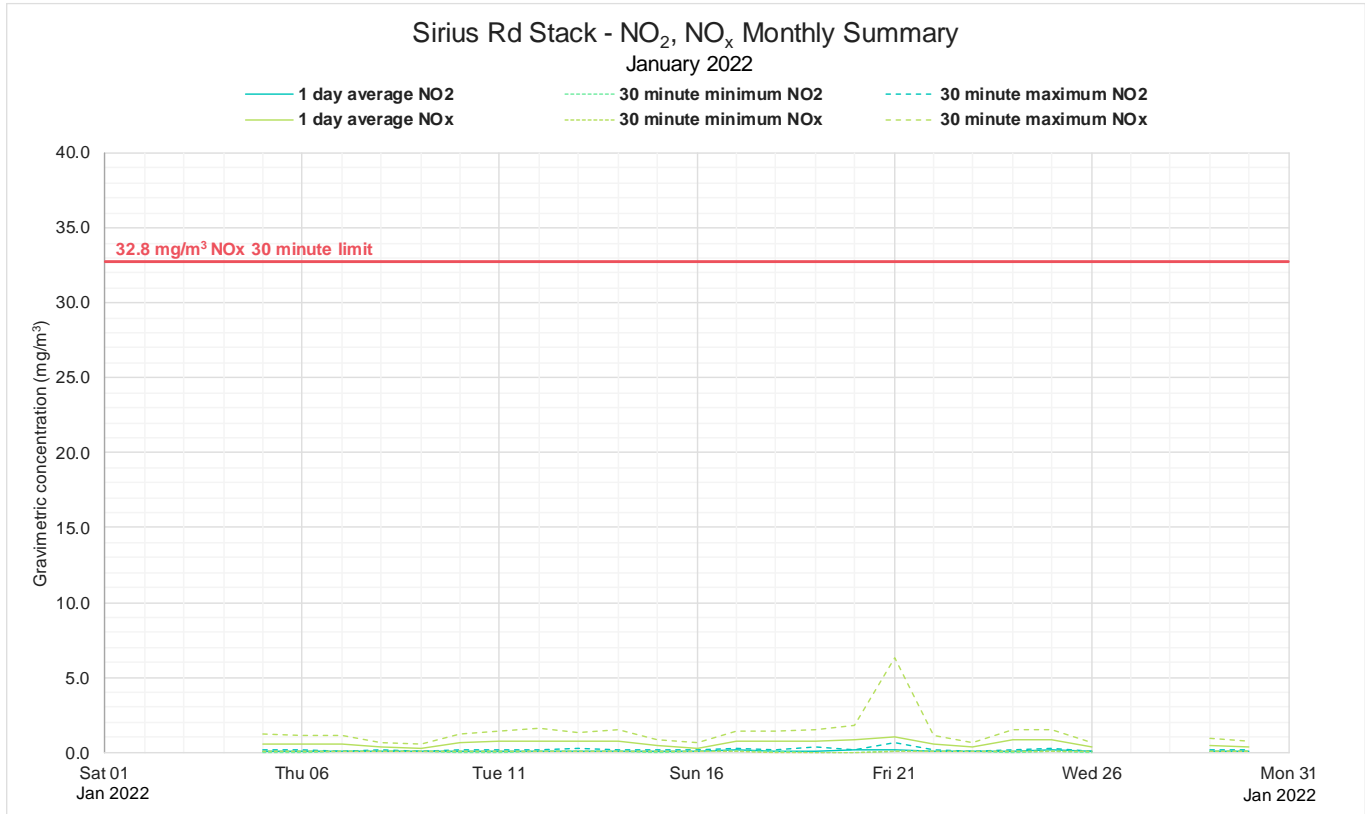


Figure 7: Sirius Rd Stack – Monthly NO<sub>x</sub>

6.4.1.7 Sirius Rd Stack – Monthly PM<sub>10</sub>

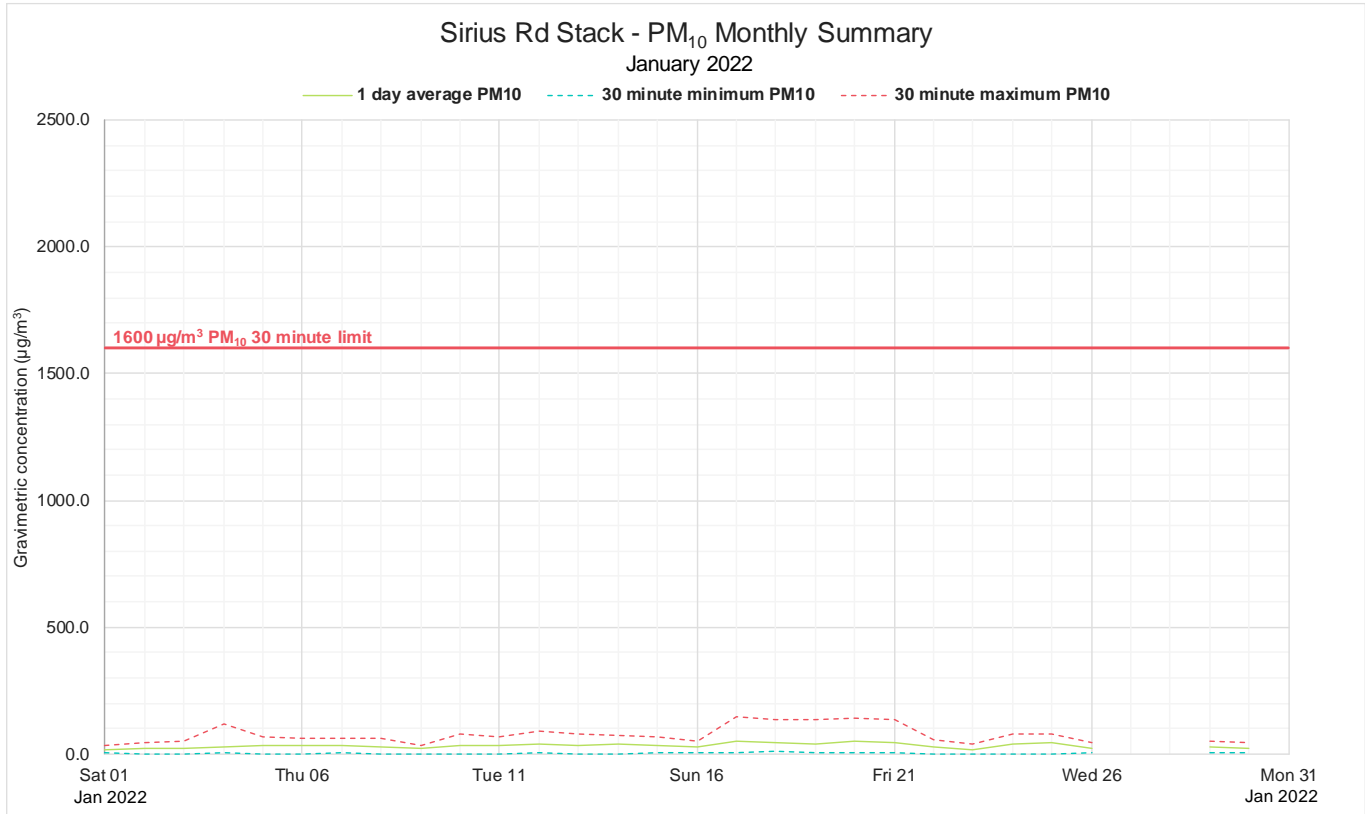


Figure 8: Sirius Rd Stack – Monthly PM<sub>10</sub>

6.4.1.8 Sirius Rd Stack – Monthly VOC

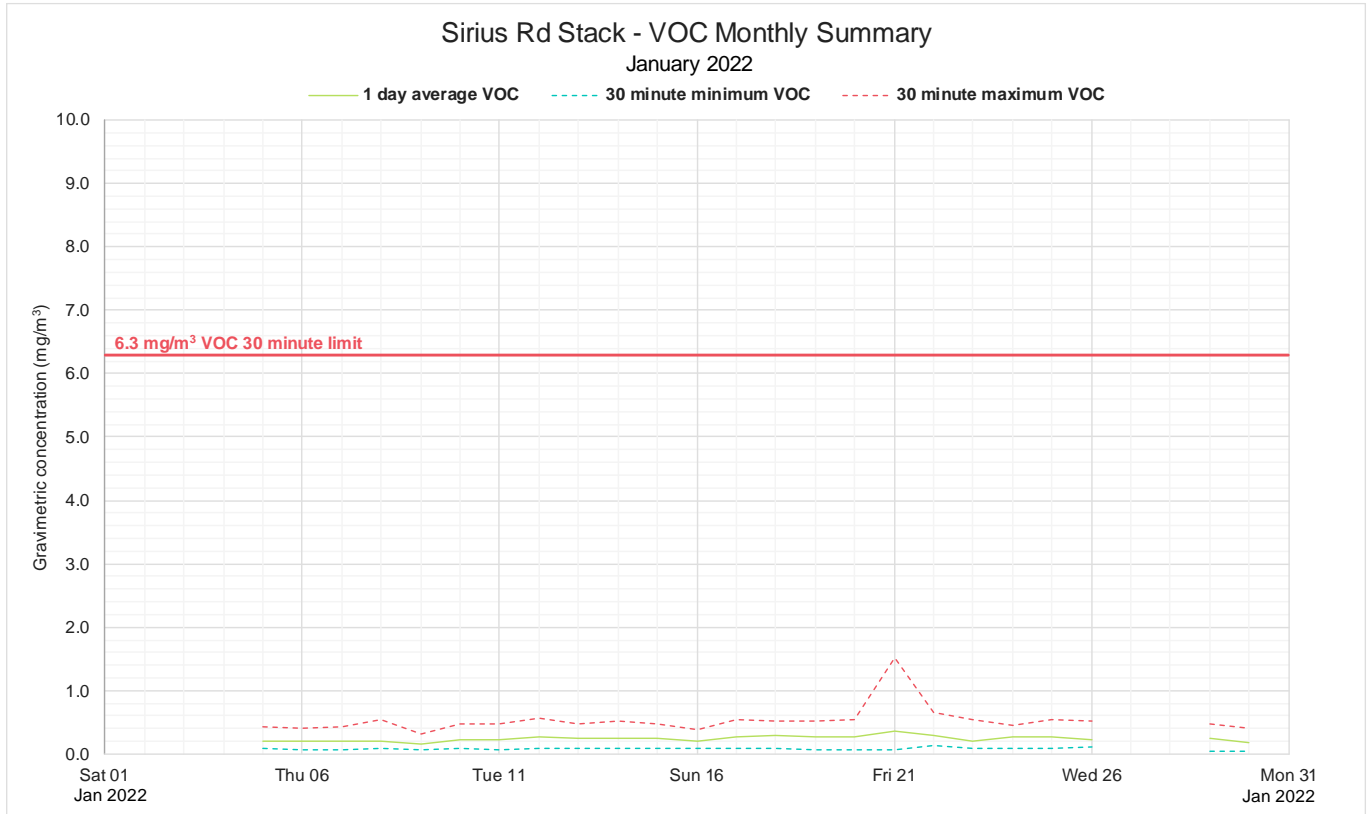


Figure 9: Sirius Rd Stack – Monthly VOC

## 6.4.2 Accumulative Loads

The following charts present annual accumulative total loads CO, NO<sub>x</sub>, PM<sub>10</sub> and VOC for the Lane Cove Tunnel ventilation stacks.

### 6.4.2.1 Combined Stacks CO Accumulative Load

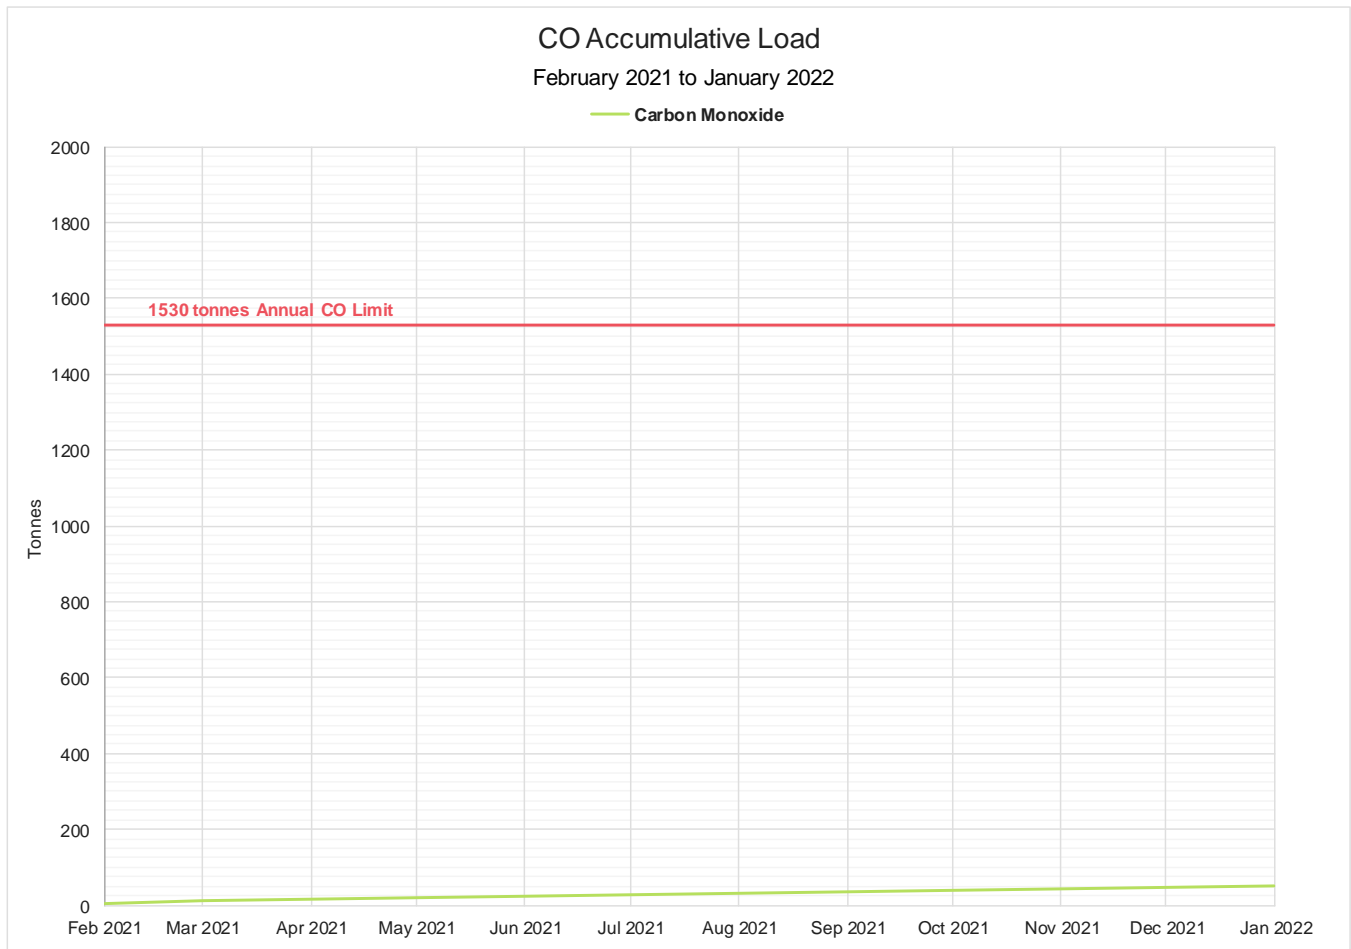


Figure 10: Combined Stacks CO Accumulative Load

6.4.2.2 Combined Stacks NO<sub>x</sub> Accumulative Load

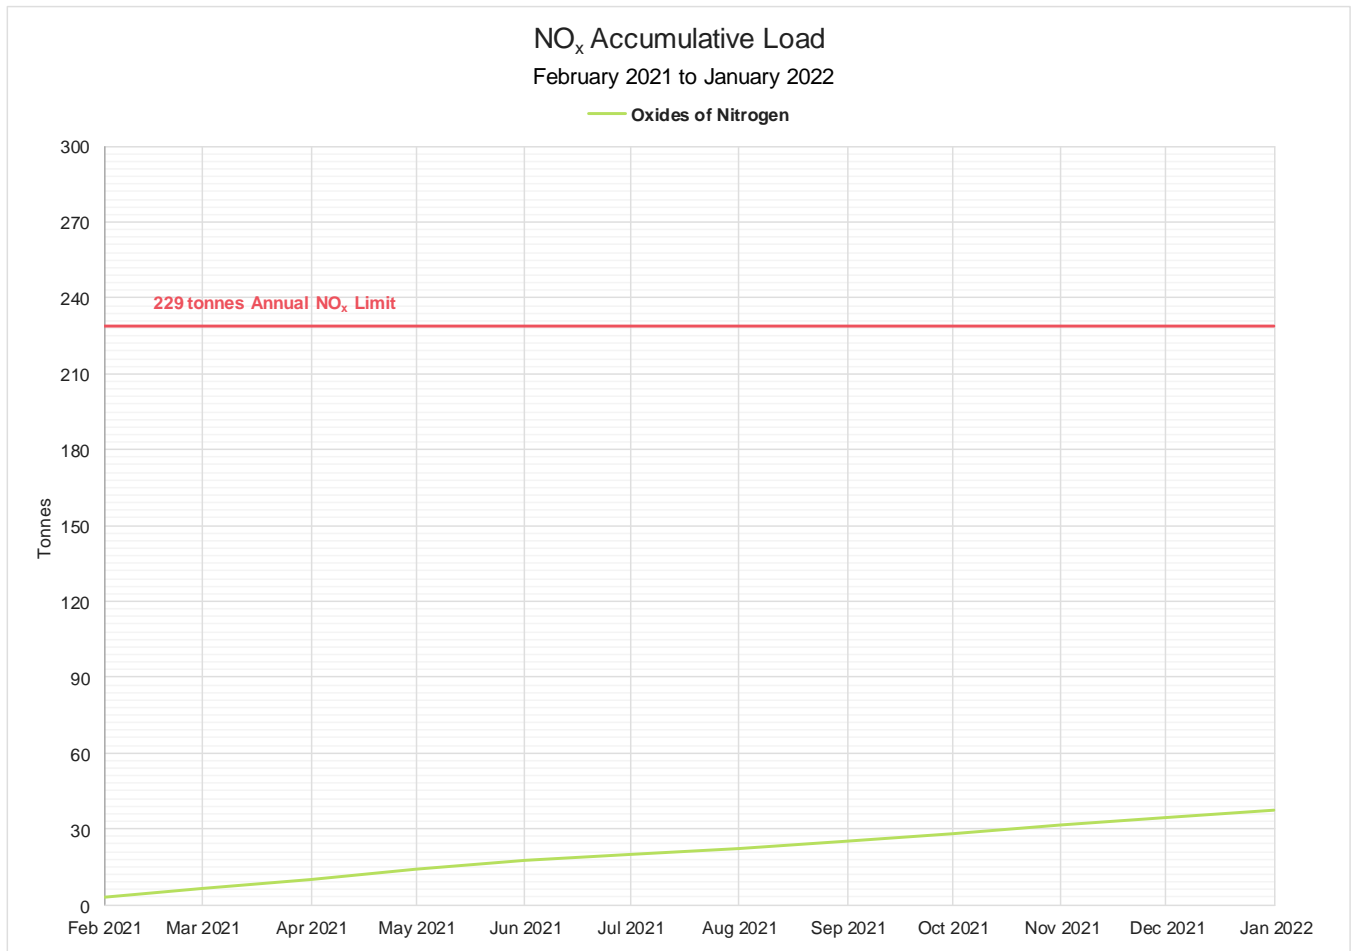


Figure 11: Combined Stacks NO<sub>x</sub> Accumulative Load



6.4.2.3 Combined Stacks PM<sub>10</sub> Accumulative Load

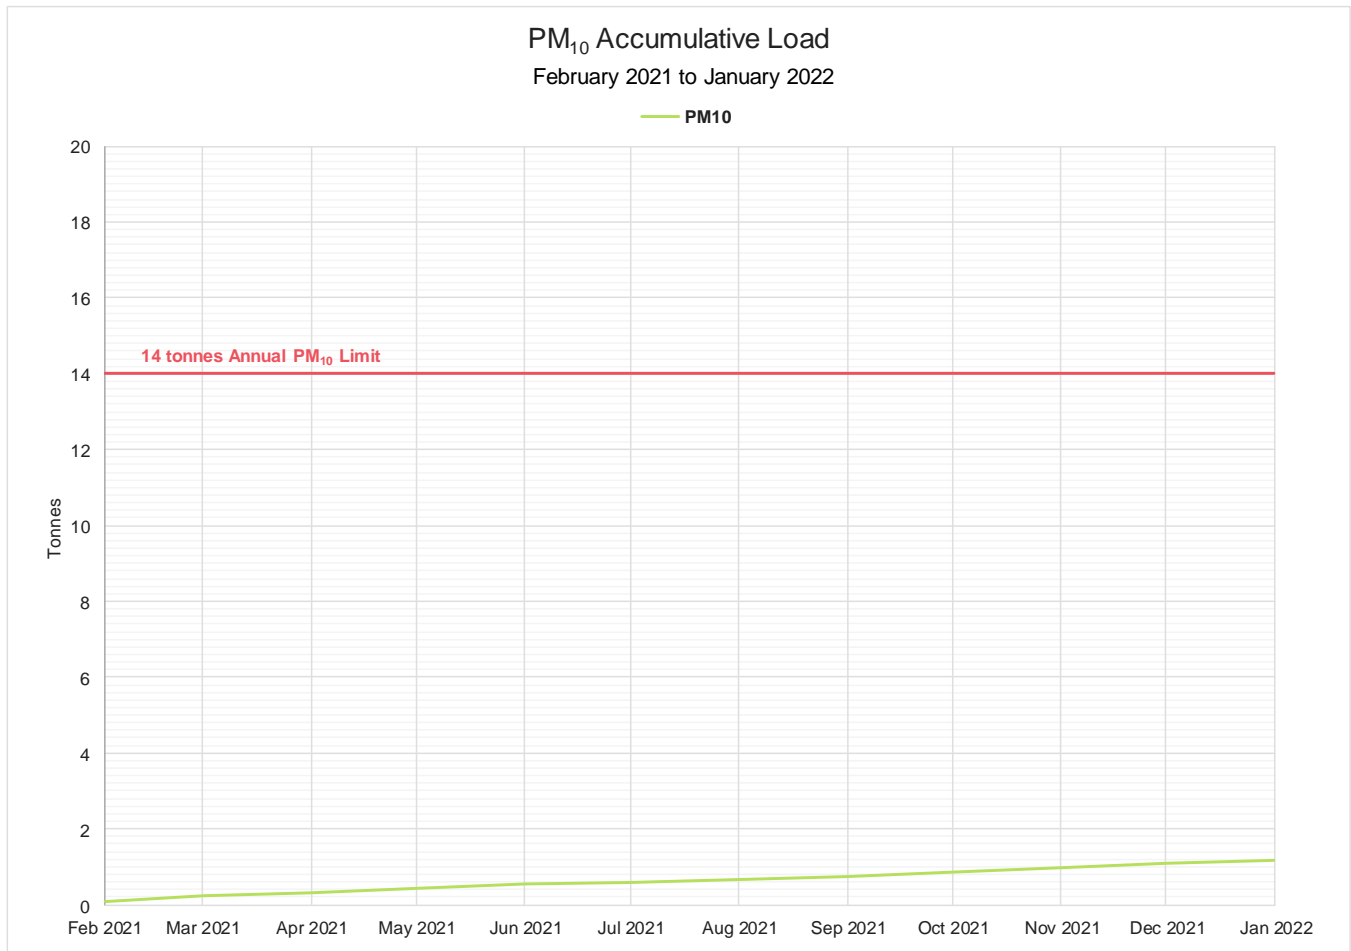


Figure 12: Combined Stacks PM<sub>10</sub> Accumulative Load

6.4.2.4 Combined Stacks VOC Accumulative Load

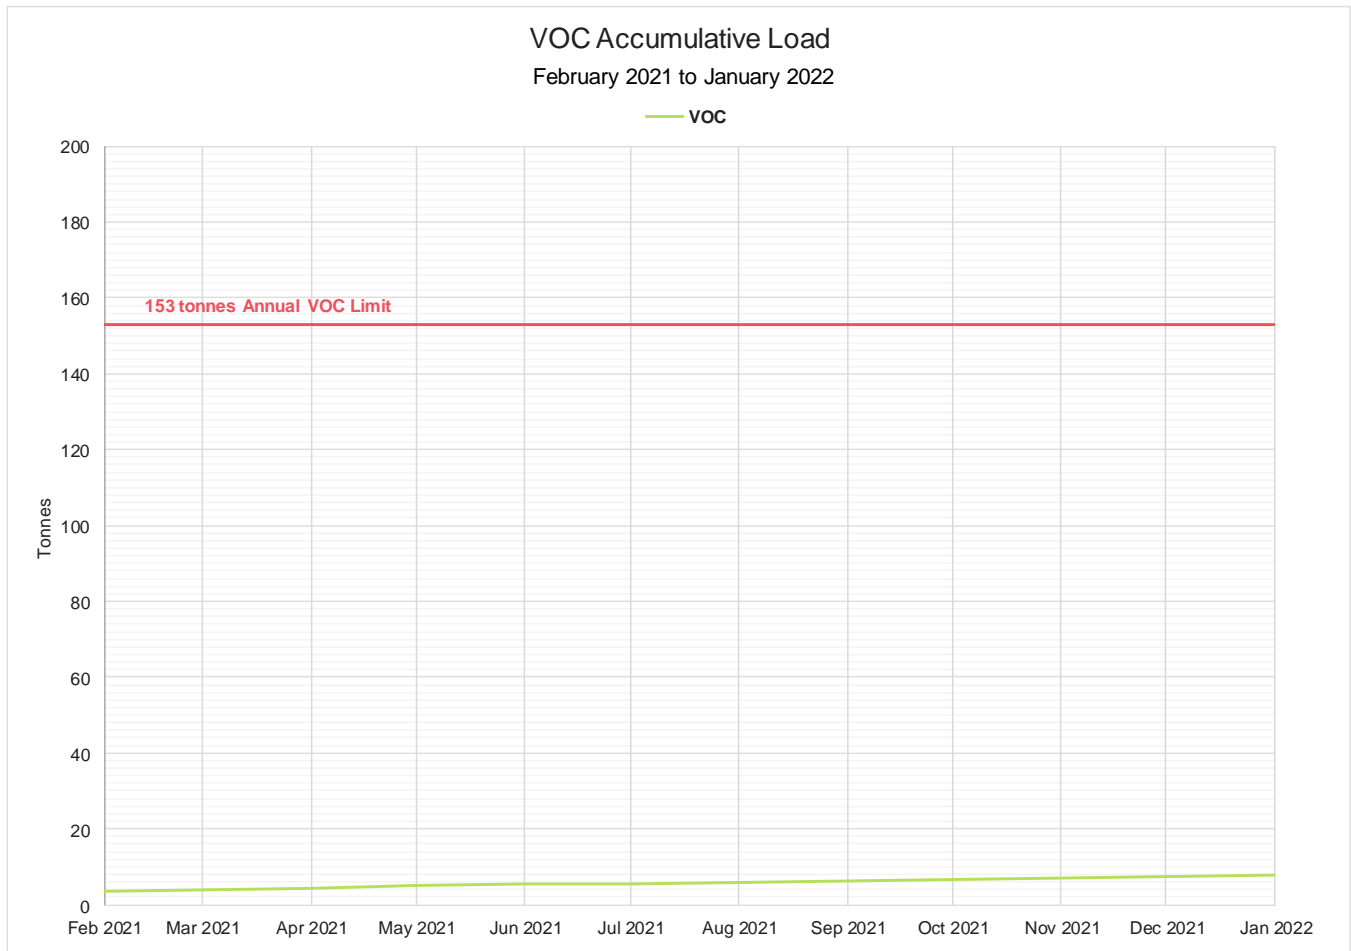


Figure 13: Combined Stacks VOC Accumulative Load

### 6.4.3 Three Monthly Trends

The following charts present 1 day average CO, NO<sub>x</sub>, PM<sub>10</sub> and VOC for the Marden St Stack, and Sirius Rd combined stack.

The daily average is calculated from 30 minute average data.

#### 6.4.3.1 Marden St Stack – Three Monthly CO

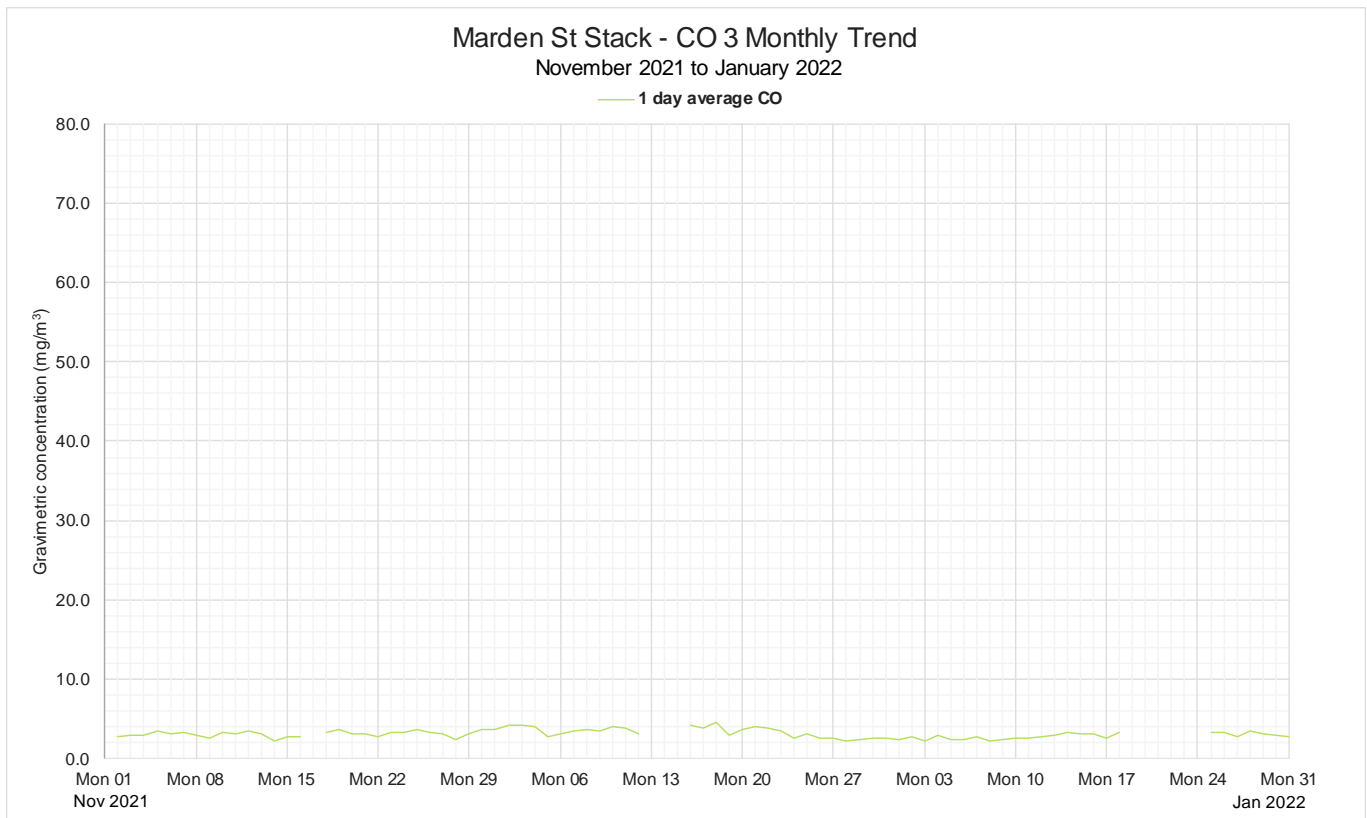


Figure 14: Marden St Stack – Three Monthly CO

6.4.3.2 Marden St Stack – Three Monthly NO<sub>2</sub>, NO<sub>x</sub>

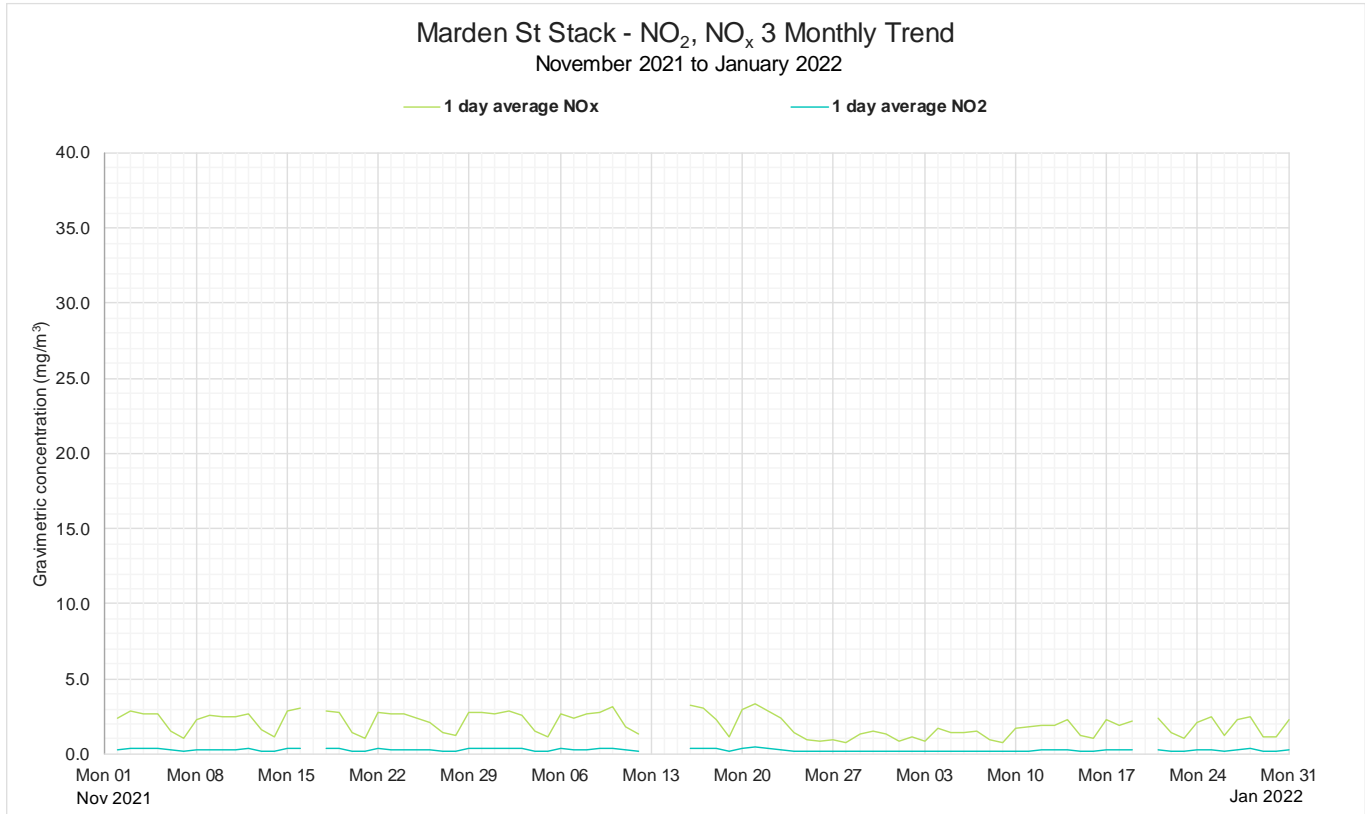


Figure 15: Marden St Stack – Three Monthly NO<sub>x</sub>

6.4.3.3 Marden St Stack – Three Monthly PM<sub>10</sub>

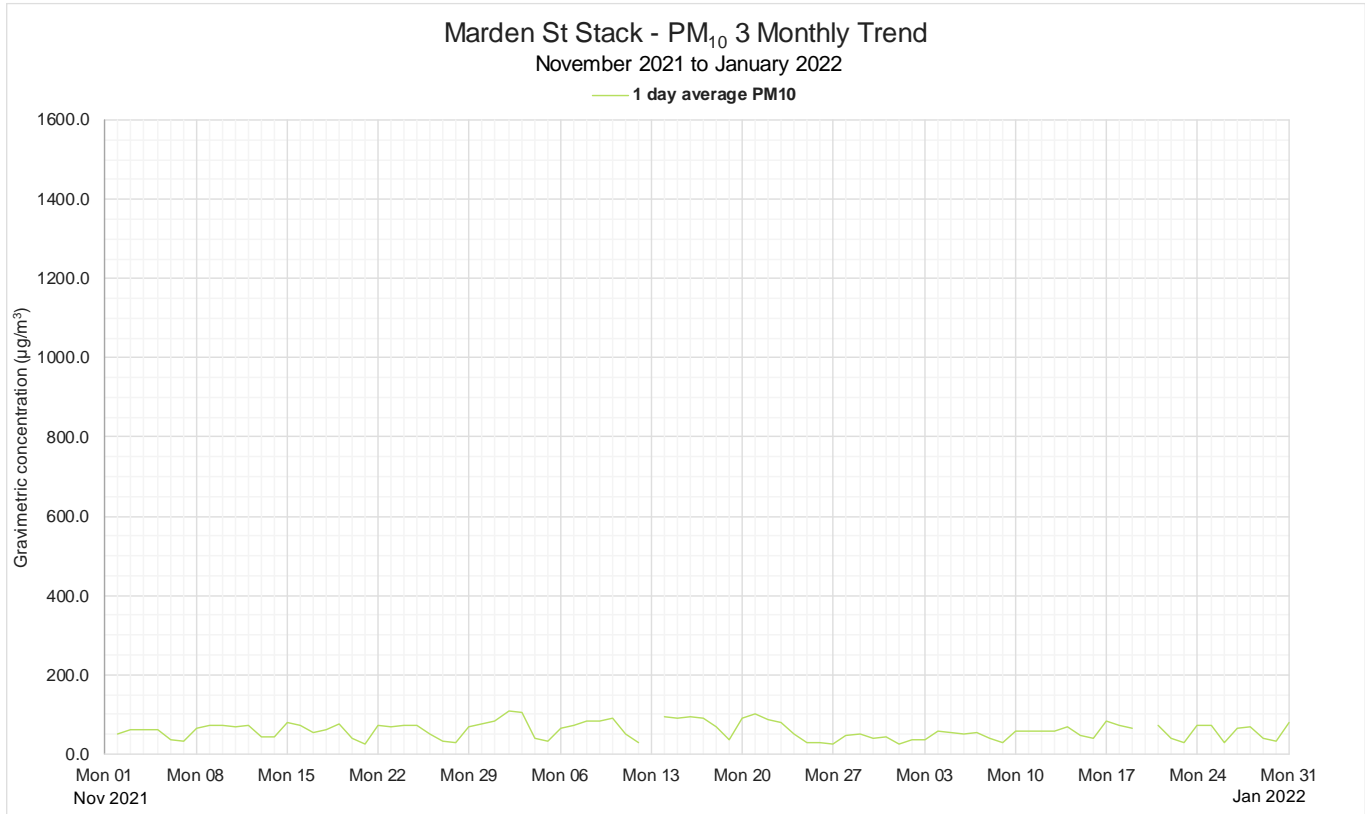


Figure 16: Marden St Stack – Three Monthly PM<sub>10</sub>

6.4.3.4 Marden St Stack – Three Monthly VOC

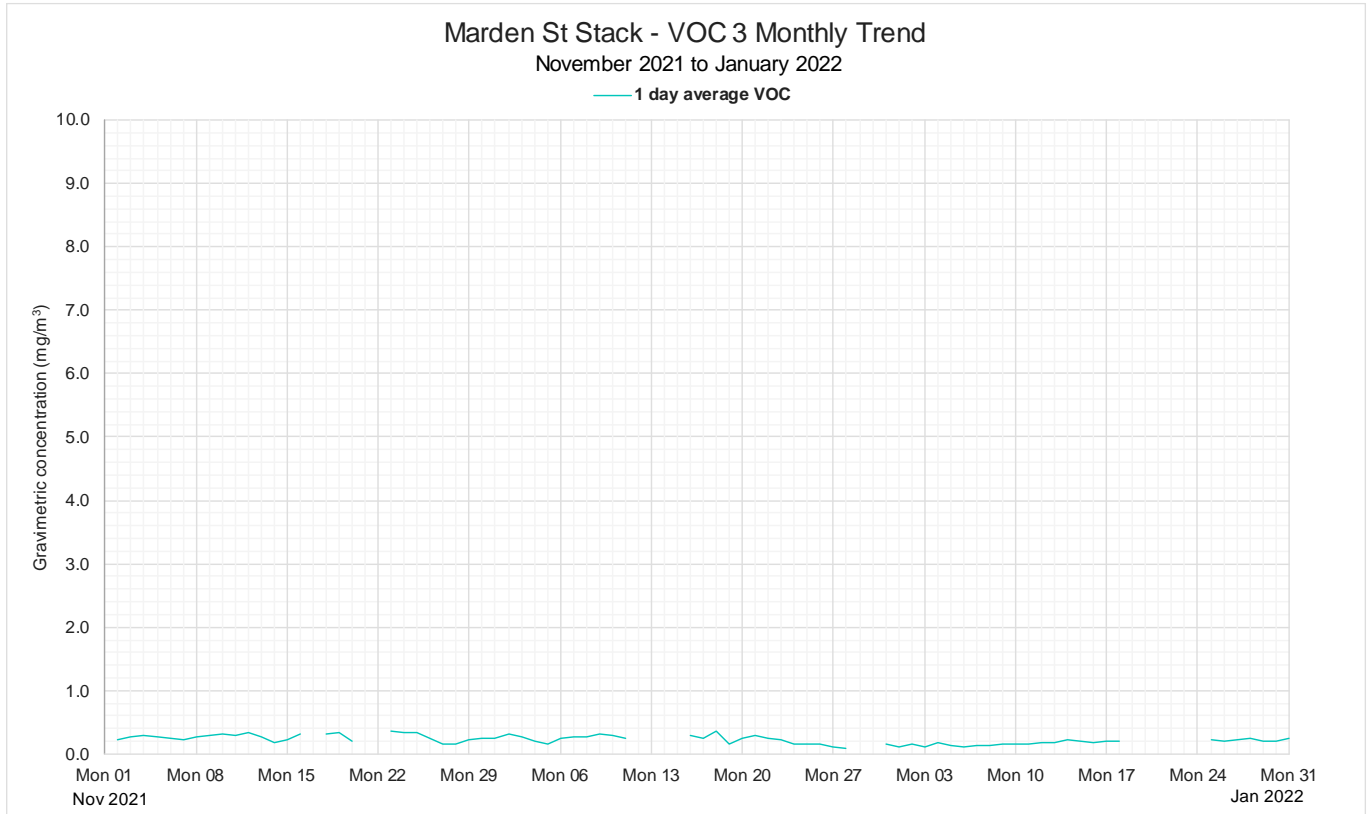


Figure 17: Marden St Stack – Three Monthly VOC

6.4.3.5 Sirius Rd Stack – Three Monthly CO

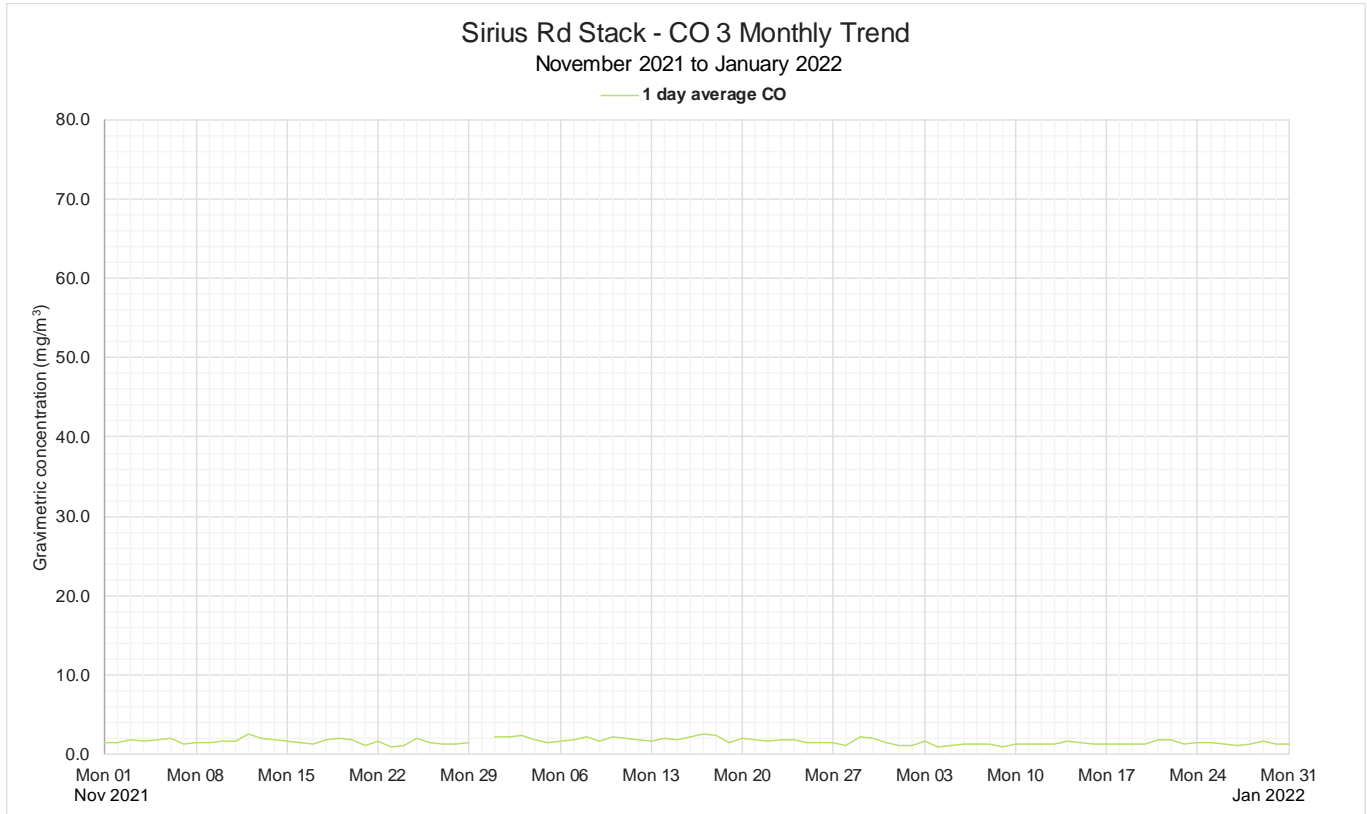


Figure 18: Sirius Rd Stack – Three Monthly CO

6.4.3.6 Sirius Rd Stack – Three Monthly NO<sub>2</sub>, NO<sub>x</sub>

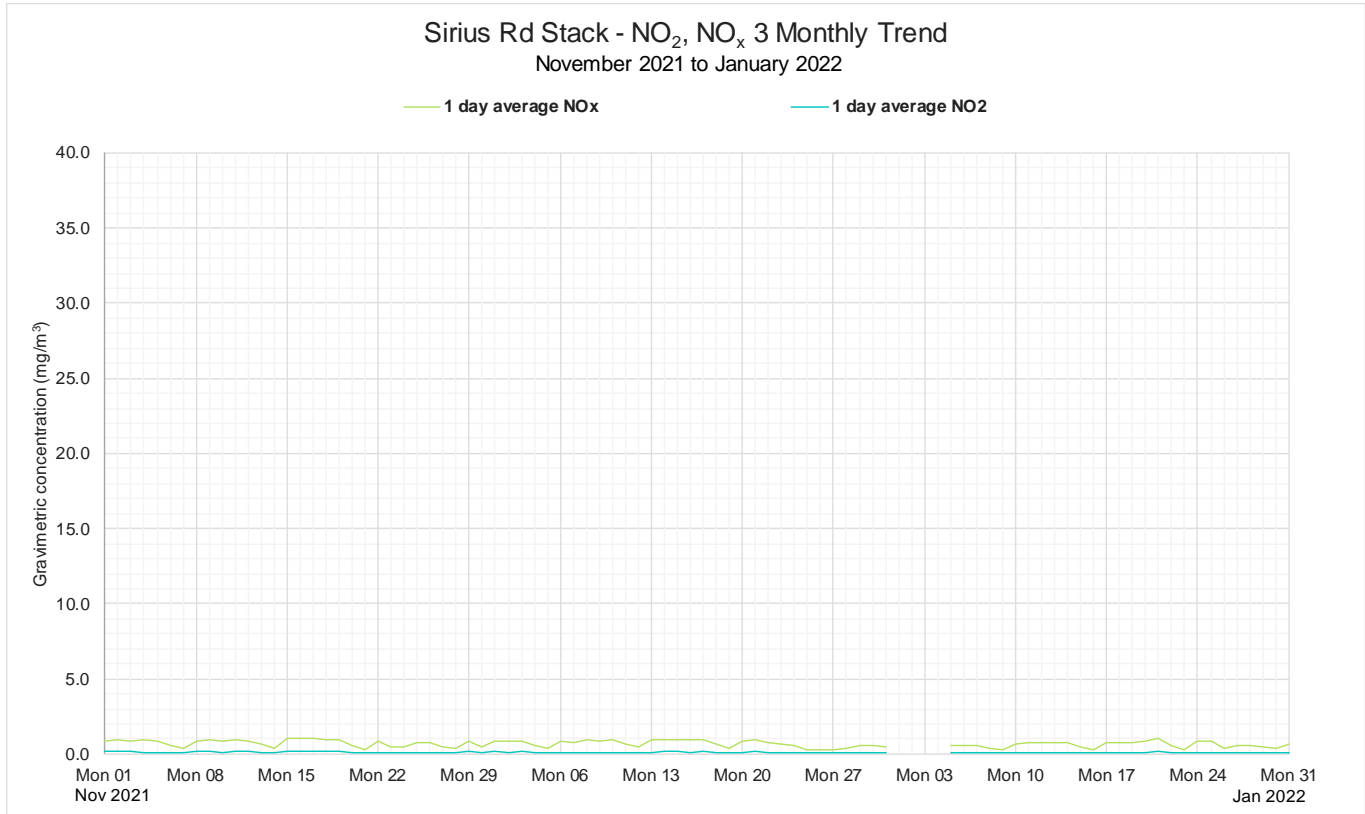


Figure 19: Sirius Rd Stack – Three Monthly NO<sub>x</sub>



6.4.3.7 Sirius Rd Stack – Three Monthly PM<sub>10</sub>

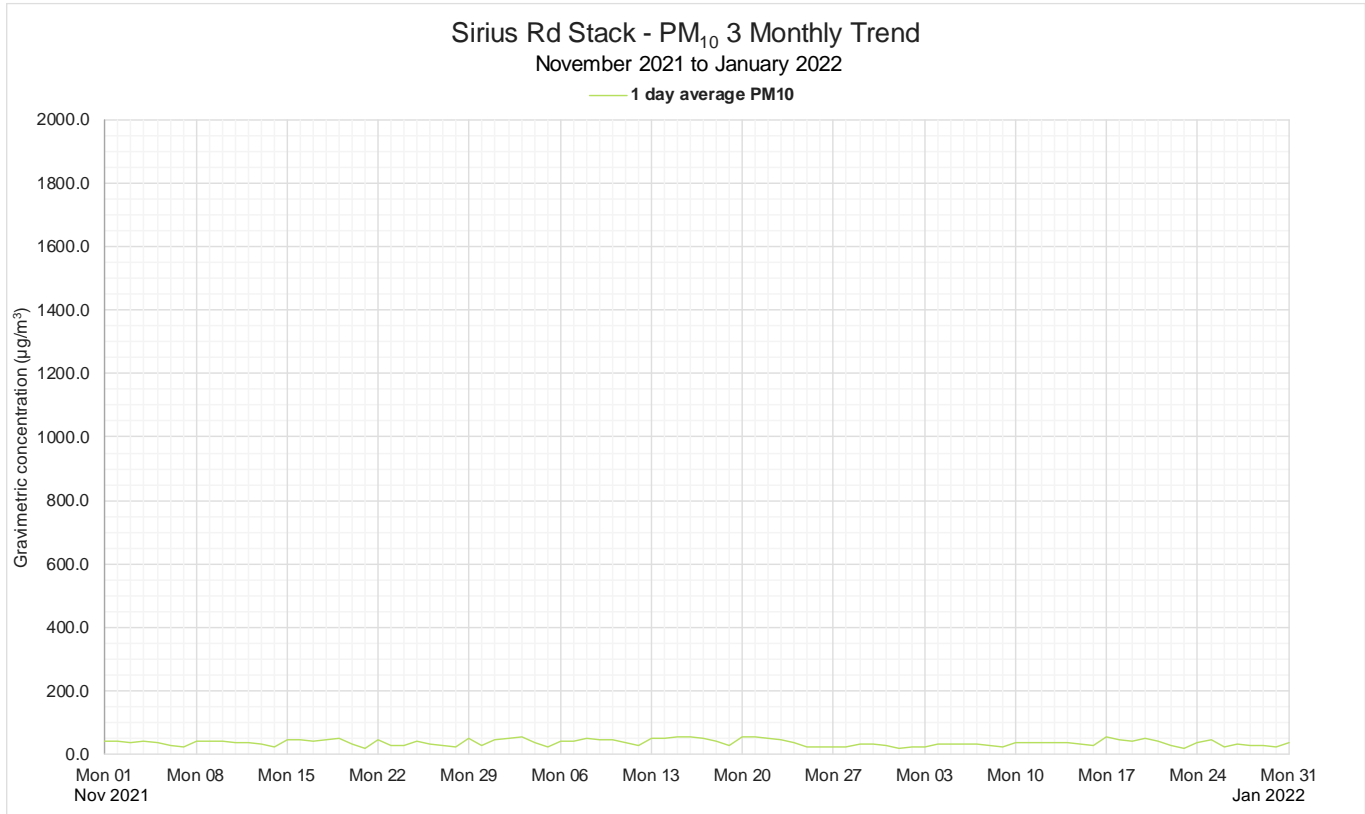


Figure 20: Sirius Rd Stack – Three Monthly PM<sub>10</sub>

6.4.3.8 Sirius Rd Stack – Three Monthly VOC

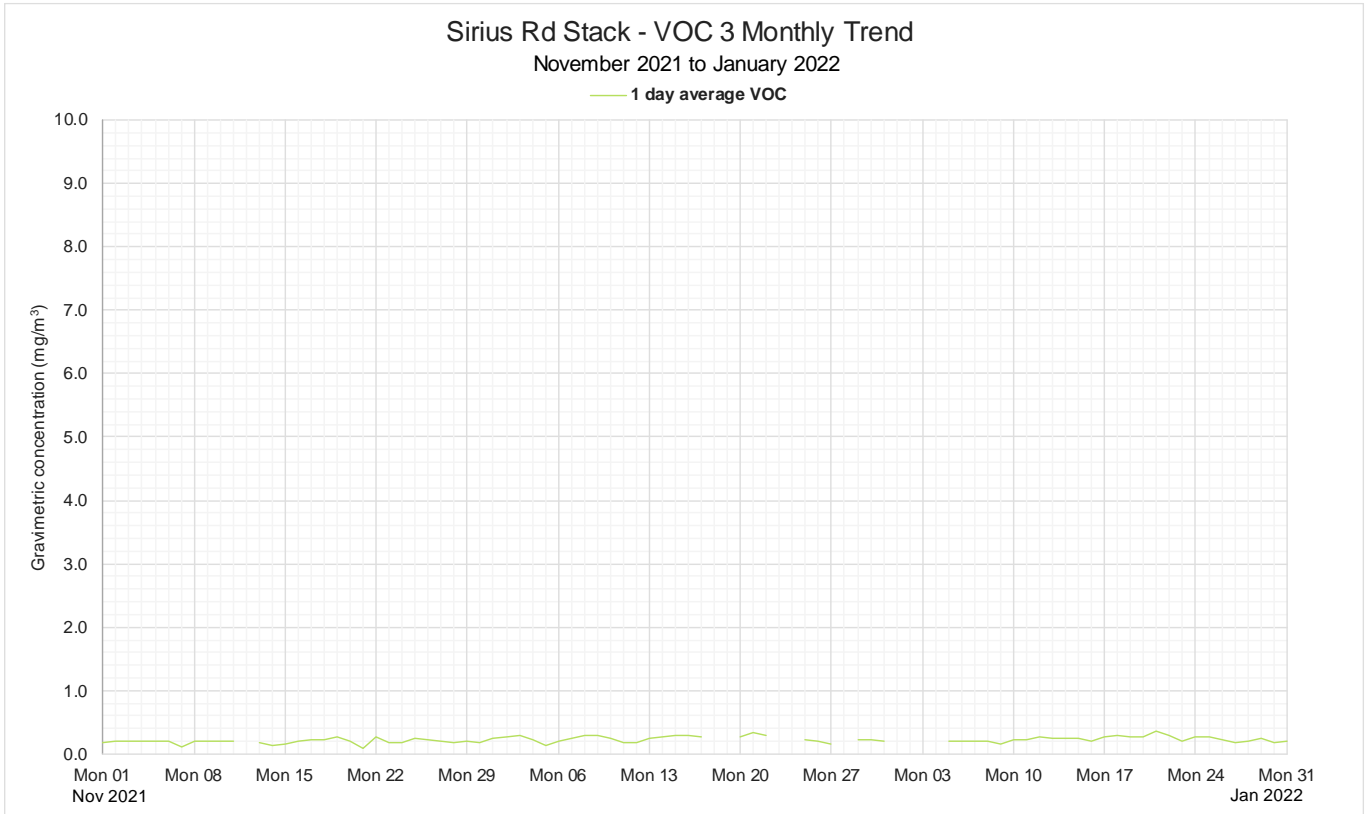


Figure 21: Sirius Rd Stack – Three Monthly VOC

## 7 Report Summary

- There were nil exceedances of the prescribed limits during the reporting period.
- Data availability for all parameters measured in the Lane Cove Tunnel Marden St stack were above 90% for the reporting period with the exception of CO and VOC.
- Data availability for all parameters measured in the Lane Cove Tunnel Sirius Rd stack were below 90% for the reporting period with the exception of PM10.

# Appendix 1

## Glossary

The following terms and abbreviations are used in this report

°C	Degrees Celsius
µg/m <sup>3</sup>	Micrograms per cubic meter at dry, standard temperature and pressure (0°C and 101.3 kPa)
CH <sub>4</sub>	Methane
CO	Carbon monoxide
eq.	Equivalents
kPa	kiloPascals
m <sup>3</sup> /s	Cubic meters per second
mg/m <sup>3</sup>	Milligrams per cubic meter at dry, standard temperature and pressure (0°C and 101.3 kPa)
NMHC	Non-methane hydrocarbons
NO	Nitric oxide
NO <sub>2</sub>	Nitrogen dioxide
NO <sub>x</sub>	Oxides of nitrogen
PM <sub>10</sub>	Particulate less than 10 microns in equivalent aerodynamic diameter
PM <sub>2.5</sub>	Particulate less than 2.5 microns in equivalent aerodynamic diameter
RH	Relative Humidity
VOC	Volatile organic compounds
ISS <sub>2.5</sub>	Isokinetic Sampling System for PM <sub>2.5</sub>
ISS <sub>10</sub>	Isokinetic Sampling System for PM <sub>10</sub>

## Data Validation Explanations

**Automatic background check** refers to when analyser samples zero air and measures the level of the concentration voltage. This voltage is taken as the zero signal level and this value is subtracted from any subsequent readings as an active zero compensation. This is the analyser's fine zero measurement.

**Calibration check outside tolerance** refers to when the calibration values are outside the tolerance limits set for the precision check.

**Offset or Multiplier Applied to data** refers to an offset or multiplier applied to the data. This operation may be performed for a number of reasons including: (a) when a clear trend / drift outside the tolerance limit can be demonstrated by repeated operation precision checks, (b) when a correction is required on previously logged data due to a calibration check being outside the allowable tolerance

**Data transmission error** refers to a period of time when the instrument could not transmit data. This may be due to a communication fault between the logger and instrument.

**Equipment malfunction/instrument fault** refers to a period of time when the instrument was not in the normal operating mode and did not measure a representative value of the existing conditions.

**Missing data/data not available** refers to a period of time when either data has been lost or could not be collected.

**Instrument Alarm** refers to an alarm produced by the instrument. A range of alarms can be produced depending on how operation of the instrument is being affected.

**Instrument out of service** refers to an unavailability of data due to an instrument being shut down for repair, maintenance, or factory calibration.

**Logger error** refers to when an error occurs and instrument readings are not correctly recorded by the logger.

**Maintenance** refers to a period of time when the logger / instrument was unavailable due to maintenance.

**Overnight span/zero out of tolerance** refers to when the span/zero reading measured by the analyser during an automatic precision check falls outside of the expected concentration limits.

**Power Interruption** refers to no power to the station therefore no data was collected at this time.

**Remote Calibration** refers to when a technician remotely connects to the station and manually performs a span check.

**Warm up after power interruption** refers to the start up period of an instrument after power has been restored.